


LB111349

7470A

INSTRUMENT ID: CV1

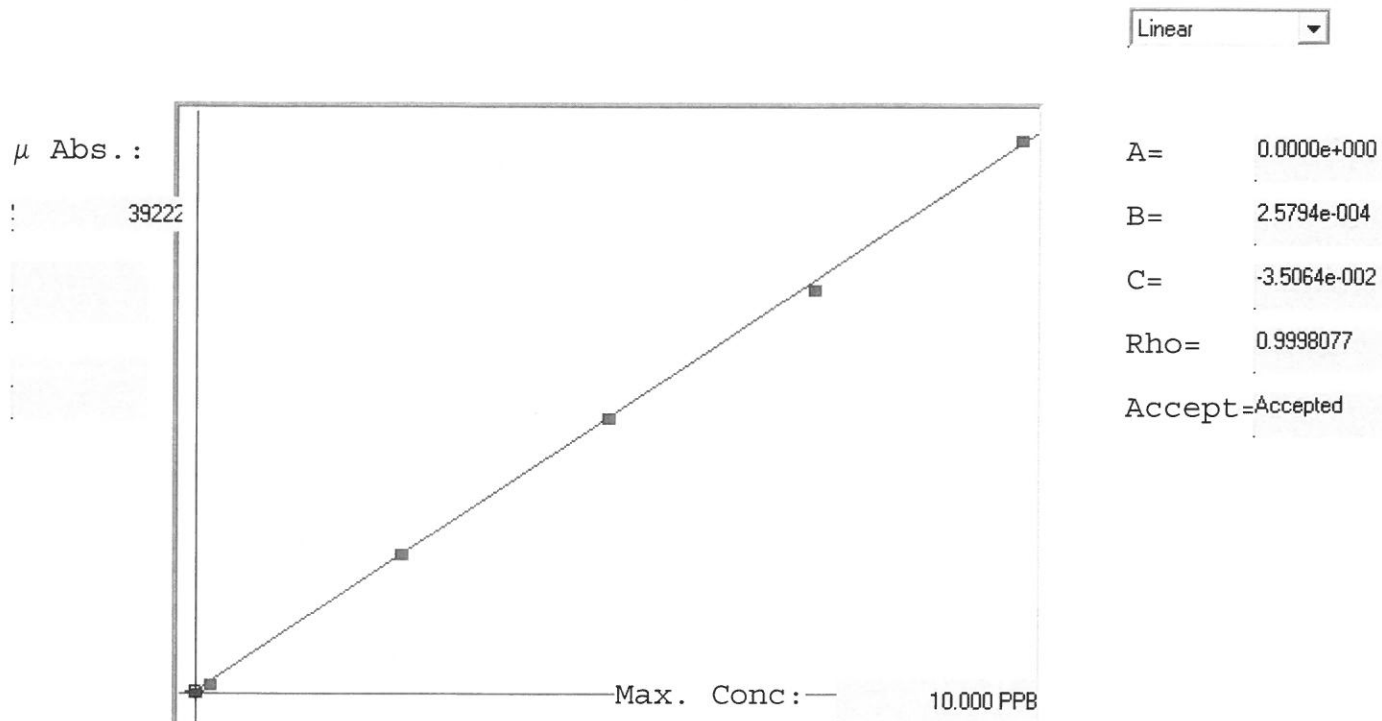

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	219	0.000	219				
0.2	0.200	0.170	-0.030	794	0.0 %	794				
2.5	2.500	2.548	0.048	10014	0.0 %	10014				
5.0	5.000	5.023	0.023	19608	0.0 %	19608				
7.5	7.500	7.357	-0.143	28657	0.0 %	28657				
10.0	10.000	10.082	0.082	39222	0.0 %	39222				

LB111349 INSTRUMENT ID ; CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Oct 2020 11:32:11

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	219	-	0.00007470A	PPB		07 Oct 2020 11:45:47	S	Std
0.2 - 1	50.2	794	-	0.20007470A	PPB		07 Oct 2020 11:48:04	S	Std
2.5 - 1	52.5	10014	-	2.50007470A	PPB		07 Oct 2020 11:50:21	S	Std
5.0 - 1	55	19608	-	5.00007470A	PPB		07 Oct 2020 11:52:38	S	Std
7.5 - 1	57.5	28657	-	7.50007470A	PPB		07 Oct 2020 11:54:54	S	Std
10.0 - 1	510	39222	-	10.00007470A	PPB		07 Oct 2020 12:02:26	S	Std
ICV46 - 1	ICV46	15265	3.9023	-7470A	PPB		07 Oct 2020 12:07:38	U	SMPL
ICB46 - 1	ICB46	21	-0.0296	-7470A	PPB		07 Oct 2020 12:09:52	U	SMPL
CCV69 - 1	CCV69	18020	4.6130	-7470A	PPB		07 Oct 2020 12:12:08	U	SMPL
CCB69 - 1	CCB69	108	-0.0072	-7470A	PPB		07 Oct 2020 12:14:23	U	SMPL
CRA - 1	CRA	760	0.1610	-7470A	PPB		07 Oct 2020 12:21:46	U	SMPL
HighStd - 1	HighStd	39322	10.1075	-7470A	PPB		07 Oct 2020 12:24:00	U	SMPL
ChkStd - 1	ChkStd	25507	6.5441	-7470A	PPB		07 Oct 2020 12:26:15	U	SMPL
PB132159BL - 1	PBW	11	-0.0322	-7470A	PPB		07 Oct 2020 12:28:32	U	SMPL
PB132159BS - 1	LCSW	13272	3.3883	-7470A	PPB		07 Oct 2020 12:30:49	U	SMPL
L4129-20 - 1	DRUM-COMP-1	87	-0.0126	-7470A	PPB		07 Oct 2020 12:33:05	U	SMPL
L4129-21 - 1	DRUM-COMP-2	189	0.0137	-7470A	PPB		07 Oct 2020 12:35:22	U	SMPL
L4129-22 - 1	DRUM-COMP-3	770	0.1635	-7470A	PPB		07 Oct 2020 12:41:04	U	SMPL
L4230-08 - 1	24702	164	0.0072	-7470A	PPB		07 Oct 2020 12:43:20	U	SMPL
L4230-10 - 1	2015	135	-0.0002	-7470A	PPB		07 Oct 2020 12:45:36	U	SMPL
CCV70 - 1	CCV70	18097	4.6328	-7470A	PPB		07 Oct 2020 12:47:52	U	SMPL
CCB70 - 1	CCB70	58	-0.0201	-7470A	PPB		07 Oct 2020 12:50:08	U	SMPL
L4230-12 - 1	27080	179	0.0111	-7470A	PPB		07 Oct 2020 12:52:23	U	SMPL
L4231-02 - 1	337	179	0.0111	-7470A	PPB		07 Oct 2020 12:54:38	U	SMPL
L4242-04 - 1	PAV-B24-100120-0-10	170	0.0088	-7470A	PPB		07 Oct 2020 12:56:54	U	SMPL
L4242-06 - 1	PAV-B24-100120-10-18	40	-0.0247	-7470A	PPB		07 Oct 2020 12:59:10	U	SMPL
L4242-12 - 1	PAV-B17-100120-0-10	-23	-0.0410	-7470A	PPB		07 Oct 2020 13:01:26	U	SMPL
L4242-14 - 1	PAV-B17-100120-10-19	211	0.0194	-7470A	PPB		07 Oct 2020 13:03:42	U	SMPL
L4242-20 - 1	PAV-B24-100120-DP	177	0.0106	-7470A	PPB		07 Oct 2020 13:06:00	U	SMPL
L4247-11 - 1	B-18(0-1)	690	0.1429	-7470A	PPB		07 Oct 2020 13:08:20	U	SMPL
L4247-13 - 1	B-19(4-5)	131	-0.0013	-7470A	PPB		07 Oct 2020 13:10:39	U	SMPL
L4247-13DUP - 1	B-19(4-5)DUP	175	0.0101	-7470A	PPB		07 Oct 2020 13:12:55	U	SMPL
CCV71 - 1	CCV71	18076	4.6274	-7470A	PPB		07 Oct 2020 13:15:11	U	SMPL
CCB71 - 1	CCB71	38	-0.0253	-7470A	PPB		07 Oct 2020 13:17:26	U	SMPL
L4247-13MS - 1	B-19(4-5)MS	12995	3.3168	-7470A	PPB		07 Oct 2020 13:19:42	U	SMPL
L4247-13MSD - 1	B-19(4-5)MSD	13983	3.5717	-7470A	PPB		07 Oct 2020 13:21:58	U	SMPL
L4248-03 - 1	NP-SOIL	108	-0.0072	-7470A	PPB		07 Oct 2020 13:24:13	U	SMPL
PB132160BL - 1	PB132160BL	124	-0.0031	-7470A	PPB		07 Oct 2020 13:26:29	U	SMPL
PB132160BS - 1	PB132160BS	14100	3.6018	-7470A	PPB		07 Oct 2020 13:31:20	U	SMPL
L4269-01 - 1	362-CONCRETE	63	-0.0188	-7470A	PPB		07 Oct 2020 13:33:36	U	SMPL
L4269-01DUP - 1	362-CONCRETEDUP	126	-0.0026	-7470A	PPB		07 Oct 2020 13:35:52	U	SMPL
L4269-01MS - 1	362-CONCRETEMS	13772	3.5172	-7470A	PPB		07 Oct 2020 13:38:09	U	SMPL
L4269-01MSD - 1	362-CONCRETEMSD	12546	3.2010	-7470A	PPB		07 Oct 2020 13:40:26	U	SMPL
L4274-02 - 1	WC-1	72	-0.0165	-7470A	PPB		07 Oct 2020 13:42:42	U	SMPL
CCV72 - 1	CCV72	18082	4.6289	-7470A	PPB		07 Oct 2020 13:44:57	U	SMPL
CCB72 - 1	CCB72	39	-0.0250	-7470A	PPB		07 Oct 2020 13:47:13	U	SMPL
PB132170BL - 1	PBW	190	0.0139	-7470A	PPB		07 Oct 2020 13:49:29	U	SMPL
PB132170BS - 1	LCSW	13723	3.5046	-7470A	PPB		07 Oct 2020 13:54:47	U	SMPL
L4221-09 - 1	OK-01-100620	1	-0.0348	-7470A	PPB		07 Oct 2020 13:57:02	U	SMPL
L4221-09DUP - 1	OK-01-100620DUP	89	-0.0121	-7470A	PPB		07 Oct 2020 13:59:18	U	SMPL
L4221-09MS - 1	OK-01-100620MS	15750	4.0274	-7470A	PPB		07 Oct 2020 14:01:34	U	SMPL
L4221-09MSD - 1	OK-01-100620MSD	15230	3.8933	-7470A	PPB		07 Oct 2020 14:03:50	U	SMPL
L4224-05 - 1	OR-02-100620	140	0.0010	-7470A	PPB		07 Oct 2020 14:06:06	U	SMPL
L4225-04 - 1	SU-04-100620	147	0.0029	-7470A	PPB		07 Oct 2020 14:08:23	U	SMPL
L4279-04 - 1	S-2	177	0.0106	-7470A	PPB		07 Oct 2020 14:10:40	U	SMPL
PB132171BL - 1	PBW	233	0.0250	-7470A	PPB		07 Oct 2020 14:12:55	U	SMPL
CCV73 - 1	CCV73	18763	4.8046	-7470A	PPB		07 Oct 2020 14:15:11	U	SMPL
CCB73 - 1	CCB73	41	-0.0245	-7470A	PPB		07 Oct 2020 14:17:26	U	SMPL
PB132171BS - 1	LCSW	15575	3.9823	-7470A	PPB		07 Oct 2020 14:19:42	U	SMPL
L4280-02 - 1	10-6-HSFRAC	154	0.0047	-7470A	PPB		07 Oct 2020 14:21:57	U	SMPL
L4280-02DUP - 1	10-6-HSFRACDUP	166	0.0078	-7470A	PPB		07 Oct 2020 14:24:13	U	SMPL
L4280-02MS - 1	10-6-HSFRACMS	12814	3.2701	-7470A	PPB		07 Oct 2020 14:26:28	U	SMPL
L4280-02MSD - 1	10-6-HSFRACMSD	13885	3.5464	-7470A	PPB		07 Oct 2020 14:28:44	U	SMPL
PB132176BL - 1	PBW	178	0.0108	-7470A	PPB		07 Oct 2020 14:31:00	U	SMPL
PB132176BS - 1	LCSW	14945	3.8198	-7470A	PPB		07 Oct 2020 14:33:17	U	SMPL
L4276-01 - 1	MW4D	250	0.0294	-7470A	PPB		07 Oct 2020 14:35:34	U	SMPL
L4276-01DUP - 1	MW4DDUP	309	0.0446	-7470A	PPB		07 Oct 2020 14:37:51	U	SMPL
L4276-01MS - 1	MW4DMS	13736	3.5080	-7470A	PPB		07 Oct 2020 14:40:07	U	SMPL
CCV74 - 1	CCV74	18761	4.8041	-7470A	PPB		07 Oct 2020 14:42:23	U	SMPL
CCB74 - 1	CCB74	24	-0.0289	-7470A	PPB		07 Oct 2020 14:44:39	U	SMPL
L4276-01MSD - 1	MW4DMSD	14436	3.6885	-7470A	PPB		07 Oct 2020 14:46:55	U	SMPL
L4276-02 - 1	MW4D	-45	-0.0467	-7470A	PPB		07 Oct 2020 14:49:11	U	SMPL
L4280-01 - 1	10-6-HSFRAC	1658	0.3926	-7470A	PPB		07 Oct 2020 14:51:27	U	SMPL
PB132159TB - 1	PB132062TB	38	-0.0253	-7470A	PPB		07 Oct 2020 14:53:43	U	SMPL
PB132160TB - 1	PB132132TB	107	-0.0075	-7470A	PPB		07 Oct 2020 14:56:00	U	SMPL
[PB132170TB - 1	PB132152TB	112	-0.0062	-7470A	PPB		07 Oct 2020 14:58:16	U	SMPL
PB132171TB - 1	PB132172TB	146	0.0026	-7470A	PPB		07 Oct 2020 15:00:32	U	SMPL
CCV75 - 1	CCV75	17850	4.5691	-7470A	PPB		07 Oct 2020 15:02:49	U	SMPL
CCB75 - 1	CCB75	79	-0.0147	-7470A	PPB		07 Oct 2020 15:05:06	U	SMPL
L4247-13LX5 - 1		138	0.0005	-7470A	PPB		07 Oct 2020 15:07:23	U	SMPL
L4247-13A - 1		16563	4.2371	-7470A	PPB		07 Oct 2020 15:09:39	U	SMPL

LB111349 INSTRUMENT ID ; CV1

Method: 7470A		Operator: Admin		Date of Analysis: 07 Oct 2020 11:32:11					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
L4269-01LX5 - 1		58	-0.0201		-7470A	PPB	07 Oct 2020 15:11:55	U	SMPL
L4269-01A - 1		16497	4.2201		-7470A	PPB	07 Oct 2020 15:14:11	U	SMPL
L4221-09LX5 - 1		46	-0.0232		-7470A	PPB	07 Oct 2020 15:16:27	U	SMPL
L4221-09A - 1		14524	3.7112		-7470A	PPB	07 Oct 2020 15:18:44	U	SMPL
L4280-02LX5 - 1		71	-0.0168		-7470A	PPB	07 Oct 2020 15:21:00	U	SMPL
L4280-02A - 1		16180	4.1384		-7470A	PPB	07 Oct 2020 15:23:16	U	SMPL
L4276-01LX5 - 1		88	-0.0124		-7470A	PPB	07 Oct 2020 15:25:32	U	SMPL
L4276-01A - 1		16363	4.1856		-7470A	PPB	07 Oct 2020 15:27:48	U	SMPL
CCV76 - 1	CCV76	18233	4.6679		-7470A	PPB	07 Oct 2020 15:30:05	U	SMPL
CCB76 - 1	CCB76	24	-0.0289		-7470A	PPB	07 Oct 2020 15:32:22	U	SMPL