


LB111402

245.1

INSTRUMENT ID: CV1

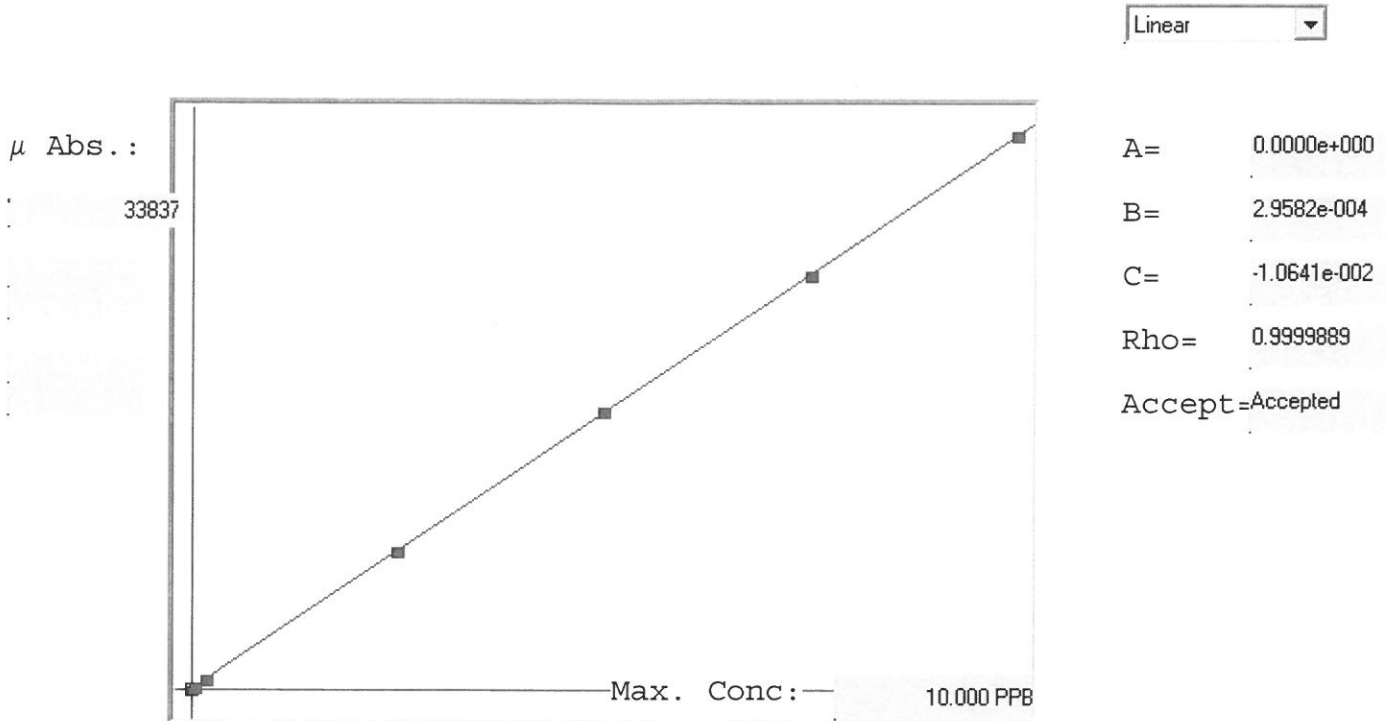

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	28	0.000	28				
0.05	0.050	0.050	0.000	205	0.0 %	205	0			
0.2	0.200	0.185	-0.015	663	0.0 %	663				
2.5	2.500	2.507	0.007	8510	0.0 %	8510				
5.0	5.000	5.036	0.036	17059	0.0 %	17059				
7.5	7.500	7.475	-0.025	25306	0.0 %	25306				
10.0	10.000	9.999	-0.001	33837	0.0 %	33837				

LB111402 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 09 Oct 2020 11:36:42

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	28	-	0.0000	245.1	PPB	09 Oct 2020 11:37:58	S	Std
0.05 - 1	50.05	205	-	0.0500	245.1	PPB	09 Oct 2020 11:40:15	S	Std
0.2 - 1	50.2	663	-	0.2000	245.1	PPB	09 Oct 2020 11:42:32	S	Std
2.5 - 1	52.5	8510	-	2.5000	245.1	PPB	09 Oct 2020 11:44:49	S	Std
5.0 - 1	55	17059	-	5.0000	245.1	PPB	09 Oct 2020 11:47:05	S	Std
7.5 - 1	57.5	25306	-	7.5000	245.1	PPB	09 Oct 2020 11:49:21	S	Std
10.0 - 1	510	33837	-	10.0000	245.1	PPB	09 Oct 2020 12:07:28	S	Std
ICV49 - 1	ICV49	13196	3.8930	-245.1		PPB	09 Oct 2020 12:12:47	U	SMPL
ICB49 - 1	ICB49	-111	-0.0435	-245.1		PPB	09 Oct 2020 12:15:02	U	SMPL
CCV95 - 1	CCV95	17025	5.0257	-245.1		PPB	09 Oct 2020 12:17:17	U	SMPL
CCB95 - 1	CCB95	-69	-0.0311	-245.1		PPB	09 Oct 2020 12:19:32	U	SMPL
CRA - 1	CRA	185	0.0441	-245.1		PPB	09 Oct 2020 12:24:22	U	SMPL
HighStd - 1	HighStd	33996	10.0460	-245.1		PPB	09 Oct 2020 12:26:36	U	SMPL
ChkStd - 1	ChkStd	25578	7.5558	-245.1		PPB	09 Oct 2020 12:28:51	U	SMPL
PB132235BL - 1	PBW	-7	-0.0127	-245.1		PPB	09 Oct 2020 12:33:41	U	SMPL
PB132235BS - 1	LCSW	12993	3.8329	-245.1		PPB	09 Oct 2020 12:35:57	U	SMPL
L4233-01 - 1	55-ST-29	4	-0.0095	-245.1		PPB	09 Oct 2020 12:38:13	U	SMPL
L4302-02 - 1	COMP	428	0.1160	-245.1		PPB	09 Oct 2020 12:40:30	U	SMPL
L4327-07 - 1	14B-(1-4)-COMP	416	0.1124	-245.1		PPB	09 Oct 2020 12:42:48	U	SMPL
L4331-01 - 1	SHELL-L15-L14	2367	0.6896	-245.1		PPB	09 Oct 2020 12:45:05	U	SMPL
L4331-01DUP - 1	SHELL-L15-L14DUP	2279	0.6635	-245.1		PPB	09 Oct 2020 12:47:20	U	SMPL
CCV96 - 1	CCV96	17049	5.0328	-245.1		PPB	09 Oct 2020 12:49:35	U	SMPL
CCB96 - 1	CCB96	-59	-0.0281	-245.1		PPB	09 Oct 2020 12:51:50	U	SMPL
L4331-01MS - 1	SHELL-L15-L14MS	15938	4.7041	-245.1		PPB	09 Oct 2020 12:54:05	U	SMPL
L4331-01MSD - 1	SHELL-L15-L14MSD	15315	4.5198	-245.1		PPB	09 Oct 2020 12:56:20	U	SMPL
L4331-02 - 1	SHELL-L15-L14	-23	-0.0174	-245.1		PPB	09 Oct 2020 12:58:36	U	SMPL
L4331-01LX5 - 1		383	0.1027	-245.1		PPB	09 Oct 2020 13:00:51	U	SMPL
L4331-01A - 1		15618	4.6095	-245.1		PPB	09 Oct 2020 13:03:07	U	SMPL
CCV97 - 1	CCV97	16599	4.8997	-245.1		PPB	09 Oct 2020 13:05:23	U	SMPL
CCB97 - 1	CCB97	-17	-0.0157	-245.1		PPB	09 Oct 2020 13:07:40	U	SMPL