


LB111462

7470A

INSTRUMENT ID: CV1

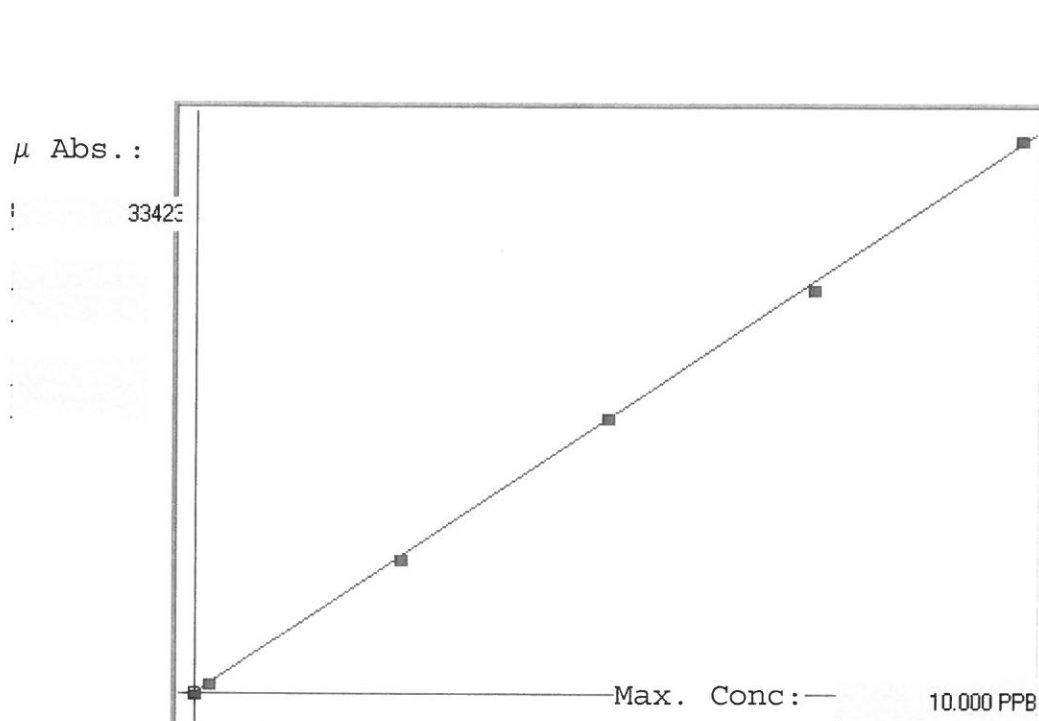

Linear

A= 0.0000e+000

B= 3.0107e-004

C= 8.8440e-003

Rho= 0.9998420

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.028	0.028	65	0.000	65				
0.2	0.200	0.203	0.003	645	0.0 %	645				
2.5	2.500	2.466	-0.034	8161	0.0 %	8161				
5.0	5.000	5.056	0.056	16764	0.0 %	16764				
7.5	7.500	7.375	-0.125	24467	0.0 %	24467				
10.0	10.000	10.072	0.072	33423	0.0 %	33423				

LB111462 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Oct 2020 08:34:00

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	65	-	0.0000	7470A	PPB	13 Oct 2020 08:44:25	S	Std
0.2 - 1	50.2	645	-	0.2000	7470A	PPB	13 Oct 2020 08:46:42	S	Std
2.5 - 1	52.5	8161	-	2.5000	7470A	PPB	13 Oct 2020 08:48:59	S	Std
5.0 - 1	55	16764	-	5.0000	7470A	PPB	13 Oct 2020 08:51:16	S	Std
7.5 - 1	57.5	24467	-	7.5000	7470A	PPB	13 Oct 2020 08:53:32	S	Std
10.0 - 1	510	33423	-	10.0000	7470A	PPB	13 Oct 2020 09:01:02	S	Std
ICV53 - 1	ICV53	12794	3.8607	-	7470A	PPB	13 Oct 2020 09:03:44	U	SMPL
ICB53 - 1	ICB53	-26	0.0010	-	7470A	PPB	13 Oct 2020 09:05:59	U	SMPL
CCV13 - 1	CCV13	16366	4.9362	-	7470A	PPB	13 Oct 2020 09:08:14	U	SMPL
CCB13 - 1	CCB13	-21	0.0025	-	7470A	PPB	13 Oct 2020 09:10:28	U	SMPL
CRA - 1	CRA	616	0.1943	-	7470A	PPB	13 Oct 2020 09:12:44	U	SMPL
HighStd - 1	HighStd	32268	9.7238	-	7470A	PPB	13 Oct 2020 09:14:59	U	SMPL
ChkStd - 1	ChkStd	22880	6.8973	-	7470A	PPB	13 Oct 2020 09:17:14	U	SMPL
PB132295BL - 1	PBW	-138	-0.0327	-	7470A	PPB	13 Oct 2020 09:19:30	U	SMPL
PB132295BS - 1	LCSW	11621	3.5076	-	7470A	PPB	13 Oct 2020 09:21:47	U	SMPL
L4225-09 - 1	SU-01-100920	-30	-0.0002	-	7470A	PPB	13 Oct 2020 09:24:03	U	SMPL
L4225-09DUP - 1	SU-01-100920DUP	50	0.0239	-	7470A	PPB	13 Oct 2020 09:26:19	U	SMPL
L4225-09MS - 1	SU-01-100920MS	11445	3.4546	-	7470A	PPB	13 Oct 2020 09:28:36	U	SMPL
L4225-09MSD - 1	SU-01-100920MSD	11136	3.3616	-	7470A	PPB	13 Oct 2020 09:30:53	U	SMPL
L4333-02 - 1	OH-WC-J6-3-6	283	0.0940	-	7470A	PPB	13 Oct 2020 09:33:09	U	SMPL
CCV14 - 1	CCV14	16522	4.9831	-	7470A	PPB	13 Oct 2020 09:35:24	U	SMPL
CCB14 - 1	CCB14	-8	0.0064	-	7470A	PPB	13 Oct 2020 09:37:39	U	SMPL
L4333-06 - 1	OH-WC-C-J4	60	0.0269	-	7470A	PPB	13 Oct 2020 09:39:55	U	SMPL
L4333-09 - 1	OH-WC-C-G2	64	0.0281	-	7470A	PPB	13 Oct 2020 09:42:10	U	SMPL
L4333-12 - 1	OH-WC-C-C1	86	0.0347	-	7470A	PPB	13 Oct 2020 09:44:26	U	SMPL
L4333-15 - 1	OH-WC-C-D4	24	0.0161	-	7470A	PPB	13 Oct 2020 09:46:41	U	SMPL
L4341-03 - 1	STOCK-PILE	79	0.0326	-	7470A	PPB	13 Oct 2020 09:48:57	U	SMPL
L4356-01 - 1	RECLAMATION-TANK	98	0.0383	-	7470A	PPB	13 Oct 2020 09:51:14	U	SMPL
PB132295TB - 1	PB132254TB	25	0.0164	-	7470A	PPB	13 Oct 2020 09:53:30	U	SMPL
L4225-09LX5 - 1		58	0.0263	-	7470A	PPB	13 Oct 2020 09:55:47	U	SMPL
L4225-09A - 1		12385	3.7376	-	7470A	PPB	13 Oct 2020 09:58:05	U	SMPL
CCV15 - 1	CCV15	15614	4.7098	-	7470A	PPB	13 Oct 2020 10:00:20	U	SMPL
CCB15 - 1	CCB15	-13	0.0049	-	7470A	PPB	13 Oct 2020 10:02:36	U	SMPL