


LB111511

7470A

INSTRUMENT IDICV1

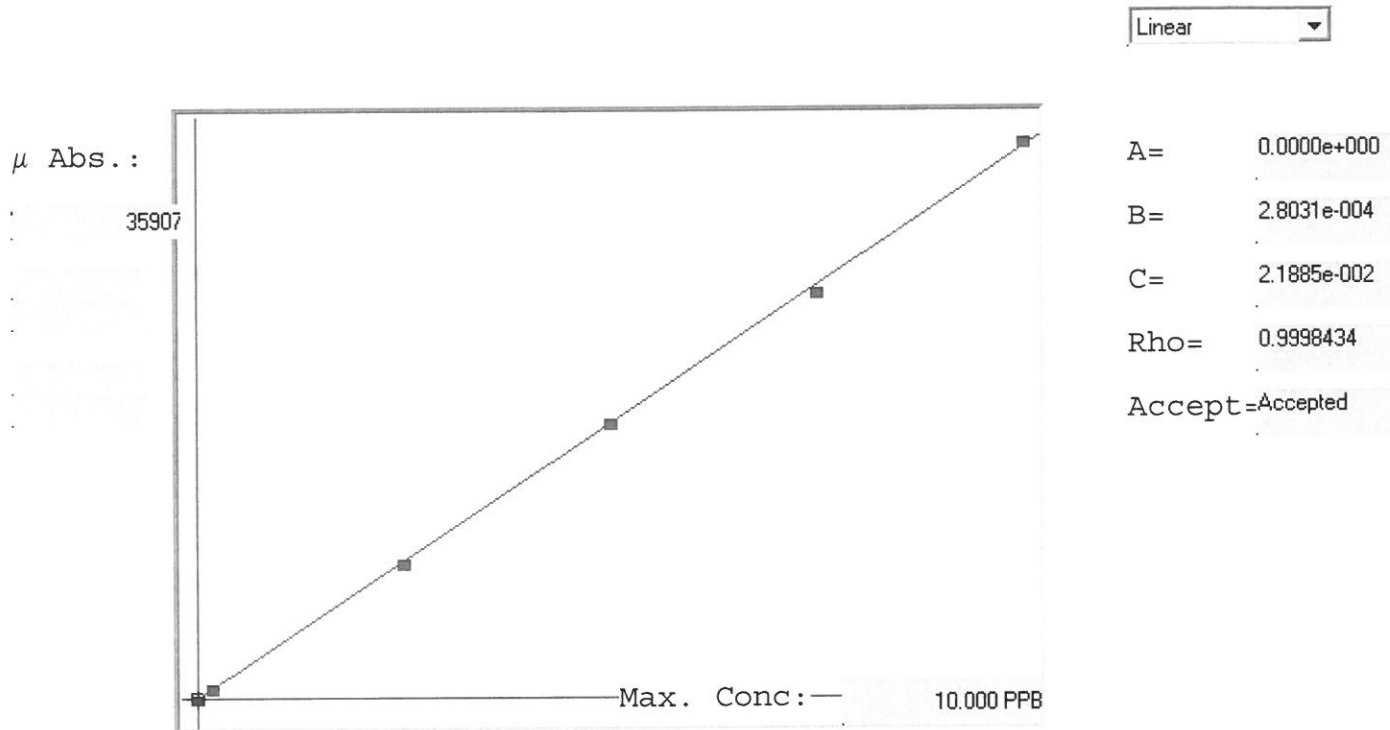

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.023	0.023	4	0.000	4				
0.2	0.200	0.216	0.016	693	0.0 %	693				
2.5	2.500	2.480	-0.020	8768	0.0 %	8768				
5.0	5.000	5.022	0.022	17837	0.0 %	17837				
7.5	7.500	7.372	-0.128	26222	0.0 %	26222				
10.0	10.000	10.087	0.087	35907	0.0 %	35907				

LB111511 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Oct 2020 09:41:38

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	4	-	0.0000	7470A	PPB	15 Oct 2020 09:46:44	S	Std
0.2 - 1	50.2	693	-	0.2000	7470A	PPB	15 Oct 2020 09:49:01	S	Std
2.5 - 1	52.5	8768	-	2.5000	7470A	PPB	15 Oct 2020 09:51:18	S	Std
5.0 - 1	55	17837	-	5.0000	7470A	PPB	15 Oct 2020 09:53:35	S	Std
7.5 - 1	57.5	26222	-	7.5000	7470A	PPB	15 Oct 2020 09:55:52	S	Std
10.0 - 1	510	35907	-	10.0000	7470A	PPB	15 Oct 2020 10:03:24	S	Std
ICV56 - 1	ICV56	13630	3.8426	-7470A	PPB	PPB	15 Oct 2020 10:09:21	U	SMPL
ICB56 - 1	ICB56	-74	0.0011	-7470A	PPB	PPB	15 Oct 2020 10:11:35	U	SMPL
CCV27 - 1	CCV27	16948	4.7726	-7470A	PPB	PPB	15 Oct 2020 10:13:51	U	SMPL
CCB27 - 1	CCB27	-51	0.0076	-7470A	PPB	PPB	15 Oct 2020 10:16:05	U	SMPL
CRA - 1	CRA	610	0.1929	-7470A	PPB	PPB	15 Oct 2020 10:18:21	U	SMPL
HighStd - 1	HighStd	33481	9.4071	-7470A	PPB	PPB	15 Oct 2020 10:20:35	U	SMPL
ChkStd - 1	ChkStd	23293	6.5512	-7470A	PPB	PPB	15 Oct 2020 10:22:50	U	SMPL
PB132370BL - 1	PBW	-117	-0.0109	-7470A	PPB	PPB	15 Oct 2020 10:25:08	U	SMPL
PB132370BS - 1	LCSW	12253	3.4566	-7470A	PPB	PPB	15 Oct 2020 10:27:24	U	SMPL
L4226-10 - 1	TR-08-101320	-46	0.0090	-7470A	PPB	PPB	15 Oct 2020 10:29:40	U	SMPL
L4226-10DUP - 1	TR-08-101320DUP	18	0.0269	-7470A	PPB	PPB	15 Oct 2020 10:31:57	U	SMPL
L4226-10MS - 1	TR-08-101320MS	11920	3.3632	-7470A	PPB	PPB	15 Oct 2020 10:34:14	U	SMPL
L4226-10MSD - 1	TR-08-101320MSD	13489	3.8030	-7470A	PPB	PPB	15 Oct 2020 10:36:31	U	SMPL
L4226-16 - 1	TR-04-101320	-50	0.0079	-7470A	PPB	PPB	15 Oct 2020 10:38:46	U	SMPL
CCV28 - 1	CCV28	16083	4.5302	-7470A	PPB	PPB	15 Oct 2020 10:41:02	U	SMPL
CCB28 - 1	CCB28	-64	0.0039	-7470A	PPB	PPB	15 Oct 2020 10:43:18	U	SMPL
PB132371BL - 1	PBW	55	0.0373	-7470A	PPB	PPB	15 Oct 2020 10:46:29	U	SMPL
PB132371BS - 1	LCSW	14312	4.0337	-7470A	PPB	PPB	15 Oct 2020 10:48:44	U	SMPL
L4381-13 - 1	DRUM-COMP	-18	0.0168	-7470A	PPB	PPB	15 Oct 2020 10:51:00	U	SMPL
L4381-13DUP - 1	DRUM-COMP DUP	48	0.0353	-7470A	PPB	PPB	15 Oct 2020 10:53:16	U	SMPL
L4381-13MS - 1	DRUM-COMP MS	13405	3.7795	-7470A	PPB	PPB	15 Oct 2020 10:55:33	U	SMPL
L4381-13MSD - 1	DRUM-COMP MSD	12655	3.5692	-7470A	PPB	PPB	15 Oct 2020 10:57:49	U	SMPL
PB132370TB - 1	PB132342TB	-61	0.0048	-7470A	PPB	PPB	15 Oct 2020 11:00:07	U	SMPL
PB132371TB - 1	PB132349TB	12	0.0252	-7470A	PPB	PPB	15 Oct 2020 11:02:24	U	SMPL
CCV29 - 1	CCV29	18586	5.2318	-7470A	PPB	PPB	15 Oct 2020 11:04:41	U	SMPL
CCB29 - 1	CCB29	-60	0.0051	-7470A	PPB	PPB	15 Oct 2020 11:06:57	U	SMPL
L4226-10LX5 - 1		26	0.0292	-7470A	PPB	PPB	15 Oct 2020 11:09:12	U	SMPL
L4226-10A - 1		13242	3.7338	-7470A	PPB	PPB	15 Oct 2020 11:11:28	U	SMPL
L4381-13LX5 - 1		32	0.0309	-7470A	PPB	PPB	15 Oct 2020 11:17:07	U	SMPL
L4381-13A - 1		13219	3.7273	-7470A	PPB	PPB	15 Oct 2020 11:19:22	U	SMPL
CCV30 - 1	CCV30	19003	5.3487	-7470A	PPB	PPB	15 Oct 2020 11:21:38	U	SMPL
CCB30 - 1	CCB30	-67	0.0031	-7470A	PPB	PPB	15 Oct 2020 11:23:53	U	SMPL