


LB 111528

7471B

INSTRUMENT ID: CV1

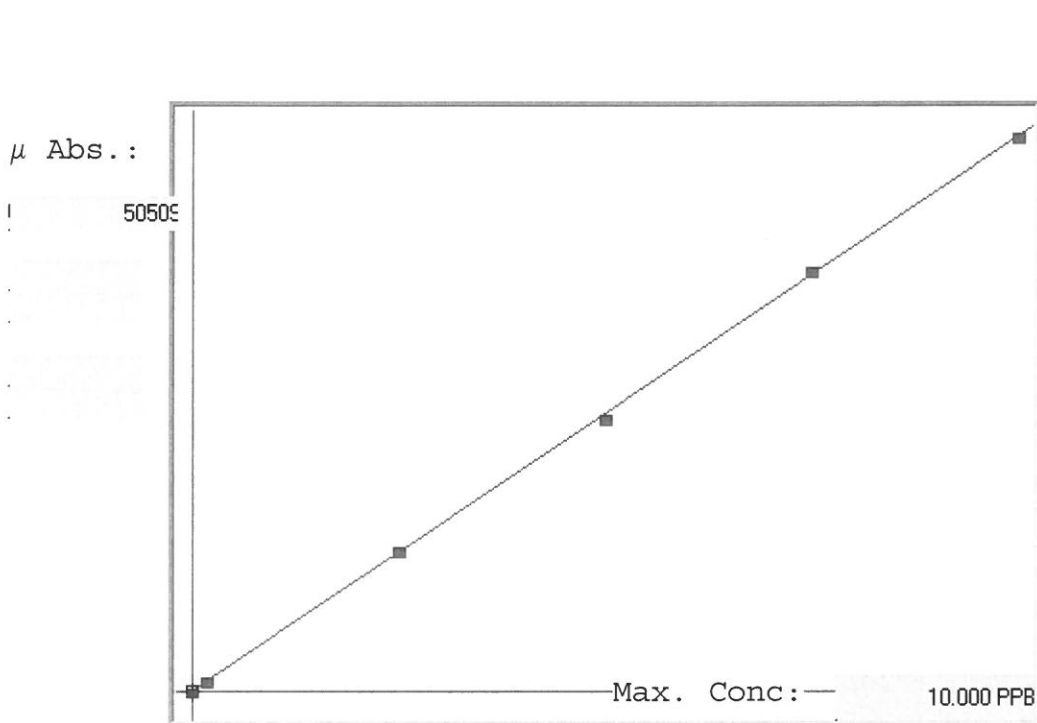

Linear

A= 0.0000e+000

B= 1.9759e-004

C= -5.8064e-003

Rho= 0.9999318

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	57	0.000	57				
0.2	0.200	0.192	-0.008	1000	0.0 %	1000				
2.5	2.500	2.527	0.027	12821	0.0 %	12821				
5.0	5.000	4.931	-0.069	24987	0.0 %	24987				
7.5	7.500	7.570	0.070	38342	0.0 %	38342				
10.0	10.000	9.974	-0.026	50509	0.0 %	50509				

LB111528 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 15 Oct 2020 14:37:14				
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50	57	-	0.0007471B	PPB		15 Oct 2020 14:38:51	S Std
0.2 - 1	50.2	1000	-	0.20007471B	PPB		15 Oct 2020 14:41:09	S Std
2.5 - 1	52.5	12821	-	2.50007471B	PPB		15 Oct 2020 14:43:26	S Std
5.0 - 1	55	24987	-	5.00007471B	PPB		15 Oct 2020 14:45:42	S Std
7.5 - 1	57.5	38342	-	7.50007471B	PPB		15 Oct 2020 14:47:59	S Std
10.0 - 1	510	50509	-	10.00007471B	PPB		15 Oct 2020 14:52:53	S Std
ICV58 - 1	ICV58	20804	4.1048	-7471B	PPB		15 Oct 2020 14:55:34	U SMPL
ICB58 - 1	ICB58	-73	-0.0202	-7471B	PPB		15 Oct 2020 14:57:49	U SMPL
CCV34 - 1	CCV34	25064	4.9465	-7471B	PPB		15 Oct 2020 15:00:05	U SMPL
CCB34 - 1	CCB34	-77	-0.0210	-7471B	PPB		15 Oct 2020 15:02:19	U SMPL
CRA - 1	CRA	982	0.1882	-7471B	PPB		15 Oct 2020 15:04:35	U SMPL
HighStd - 1	HighStd	50837	10.0389	-7471B	PPB		15 Oct 2020 15:06:50	U SMPL
ChkStd - 1	ChkStd	36208	7.1484	-7471B	PPB		15 Oct 2020 15:09:05	U SMPL
PB132385BL - 1	PBS	-94	-0.0244	-7471B	PPB		15 Oct 2020 15:11:23	U SMPL
PB132385BS - 1	LCSS	19815	3.9094	-7471B	PPB		15 Oct 2020 15:13:40	U SMPL
L4214-01 - 1	LOD-MDL-SOIL-01-QT4-2020	288	0.0511	-7471B	PPB		15 Oct 2020 15:15:56	U SMPL
L4214-02 - 1	LOQ-SOIL-02-QT4-2020	1007	0.1932	-7471B	PPB		15 Oct 2020 15:20:57	U SMPL
L4223-01 - 1	PL-01-101420	2143	0.4176	-7471B	PPB		15 Oct 2020 15:23:14	U SMPL
L4226-07 - 1	TR-08-101320	5438	1.0687	-7471B	PPB		15 Oct 2020 15:30:22	U SMPL
L4226-07DUP - 1	TR-08-101320DUP	4867	0.9558	-7471B	PPB		15 Oct 2020 15:32:36	U SMPL
CCV35 - 1	CCV35	25038	4.9413	-7471B	PPB		15 Oct 2020 15:34:52	U SMPL
CCB35 - 1	CCB35	-66	-0.0188	-7471B	PPB		15 Oct 2020 15:37:07	U SMPL
L4226-07MS - 1	TR-08-101320MS	23155	4.5693	-7471B	PPB		15 Oct 2020 15:39:23	U SMPL
L4226-07MSD - 1	TR-08-101320MSD	25776	5.0872	-7471B	PPB		15 Oct 2020 15:41:38	U SMPL
L4226-13 - 1	TR-04-101320	6667	1.3115	-7471B	PPB		15 Oct 2020 15:43:54	U SMPL
L4227-01 - 1	BU-01-101420	998	0.1914	-7471B	PPB		15 Oct 2020 15:46:09	U SMPL
L4383-02 - 1	BB-SOIL	1109	0.2133	-7471B	PPB		15 Oct 2020 15:48:25	U SMPL
L4392-02 - 1	TP-1	177	0.0292	-7471B	PPB		15 Oct 2020 15:50:41	U SMPL
L4392-06 - 1	TP-2	7310	1.4385	-7471B	PPB		15 Oct 2020 15:52:58	U SMPL
L4392-10 - 1	TP-3	13588	2.6790	-7471B	PPB		15 Oct 2020 15:55:15	U SMPL
L4392-14 - 1	TP-4	438	0.0807	-7471B	PPB		15 Oct 2020 15:57:32	U SMPL
L4393-04 - 1	SP-COMP	5697	1.1198	-7471B	PPB		15 Oct 2020 15:59:47	U SMPL
CCV36 - 1	CCV36	24966	4.9271	-7471B	PPB		15 Oct 2020 16:02:03	U SMPL
CCB36 - 1	CCB36	21	-0.0017	-7471B	PPB		15 Oct 2020 16:04:18	U SMPL
L4404-01 - 1	SHELL-L15-L14-NORTH	9761	1.9228	-7471B	PPB		15 Oct 2020 16:06:33	U SMPL
L4406-01 - 1	JC-02-101420-A	69997	13.8246	-7471B	PPB		15 Oct 2020 16:08:49	U SMPL
L4406-09 - 1	JC-02-101420-B	3189	0.6243	-7471B	PPB		15 Oct 2020 16:11:04	U SMPL
L4407-01 - 1	FK-GF-02-062-A	3526	0.6909	-7471B	PPB		15 Oct 2020 16:13:22	U SMPL
L4407-03 - 1	FK-GF-02-062-B	3080	0.6028	-7471B	PPB		15 Oct 2020 16:15:38	U SMPL
L4226-07LX5 - 1		996	0.1910	-7471B	PPB		15 Oct 2020 16:17:54	U SMPL
L4226-07A - 1		25439	5.0206	-7471B	PPB		15 Oct 2020 16:20:10	U SMPL
L4406-01DLX5 - 1		13980	2.7564	-7471B	PPB		15 Oct 2020 16:22:27	U SMPL
CCV37 - 1	CCV37	25134	4.9603	-7471B	PPB		15 Oct 2020 16:24:44	U SMPL
CCB37 - 1	CCB37	-64	-0.0185	-7471B	PPB		15 Oct 2020 16:26:59	U SMPL