


L3111687

ISM02.4

INSTRUMENT ID: CV4

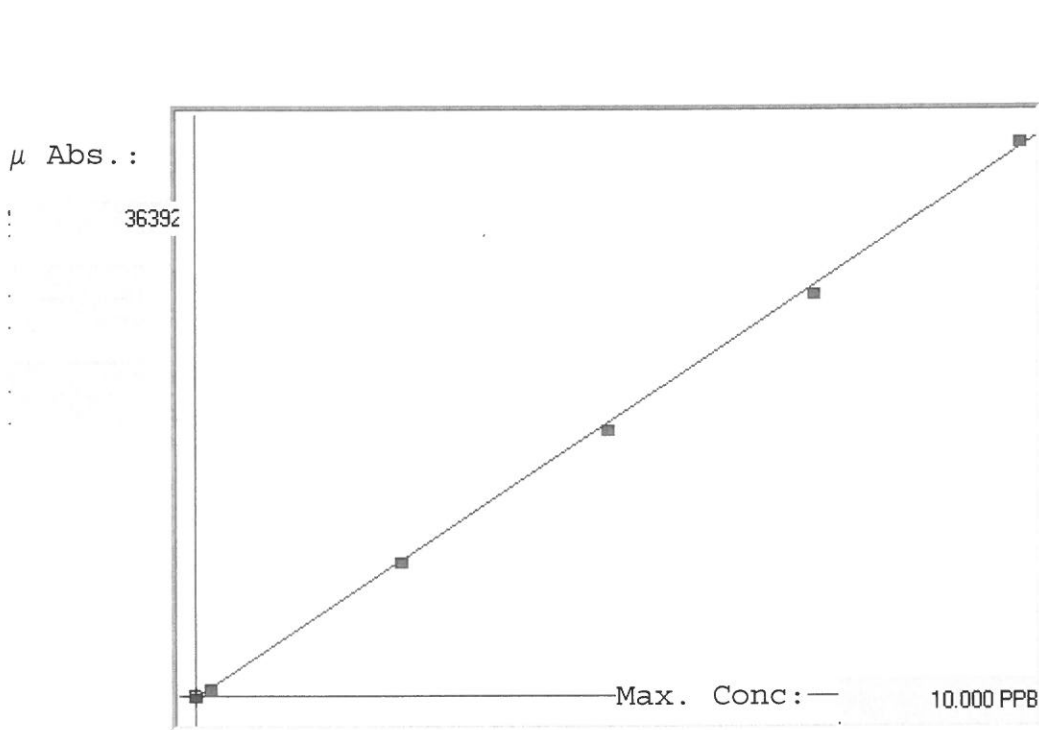

Linear

A= 0.0000e+000

B= 2.7672e-004

C= 4.9450e-002

Rho= 0.9997622

Accept=Accepted

*type
y-intercept*

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.056	0.056	23	0.000	23					2
0.05	0.050					400					1
0.20	0.200	0.204	0.004	559	0.0 %	559					-2
2.50	2.500	2.523	0.023	8937	0.0 %	8937					-2
5.00	5.000	4.911	-0.089	17568	0.0 %	17568					1
7.50	7.500	7.387	-0.113	26514	0.0 %	26514					
10.0	10.000	10.120	0.120	36392	0.0 %	36392					

LB111687

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	23	-		0 ISM02.4	PPB	10/26/2020 11:11	Std
	0.2 S0.2	559	-		0.2 ISM02.4	PPB	10/26/2020 11:13	Std
	2.5 S2.5	8937	-		2.5 ISM02.4	PPB	10/26/2020 11:16	Std
	5 S5.0	17568	-		5 ISM02.4	PPB	10/26/2020 11:18	Std
	7.5 S7.5	26514	-		7.5 ISM02.4	PPB	10/26/2020 11:20	Std
	10 S10.0	36392	-		10 ISM02.4	PPB	10/26/2020 11:25	Std
ICV	ICV	15043	4.2122 -		ISM02.4	PPB	10/26/2020 11:28	SMPL
ICB	ICB	-75	0.0287 -		ISM02.4	PPB	10/26/2020 11:30	SMPL
CCV095	CCV095	17607	4.9217 -		ISM02.4	PPB	10/26/2020 11:32	SMPL
CCB095	CCB095	-72	0.0295 -		ISM02.4	PPB	10/26/2020 11:35	SMPL
L4509-06	MC0AQ7	572	0.2077 -		ISM02.4	PPB	10/26/2020 11:44	SMPL
L4509-07	MC0ARO	465	0.1781 -		ISM02.4	PPB	10/26/2020 11:46	SMPL
L4509-08	MC0AR0D	400	0.1601 -		ISM02.4	PPB	10/26/2020 11:48	SMPL
L4509-09	MC0AR0S	4291	1.2369 -		ISM02.4	PPB	10/26/2020 11:53	SMPL
PB132607BL	PBW607	4	0.0506 -		ISM02.4	PPB	10/26/2020 11:55	SMPL
PB132607TB	LEB607	285	0.1283 -		ISM02.4	PPB	10/26/2020 11:58	SMPL
CCV096	CCV096	17480	4.8866 -		ISM02.4	PPB	10/26/2020 12:00	SMPL
CCB096	CCB096	-56	0.034 -		ISM02.4	PPB	10/26/2020 12:02	SMPL