


LB111762

7470A

INSTRUMENT ID: CXL

Linear

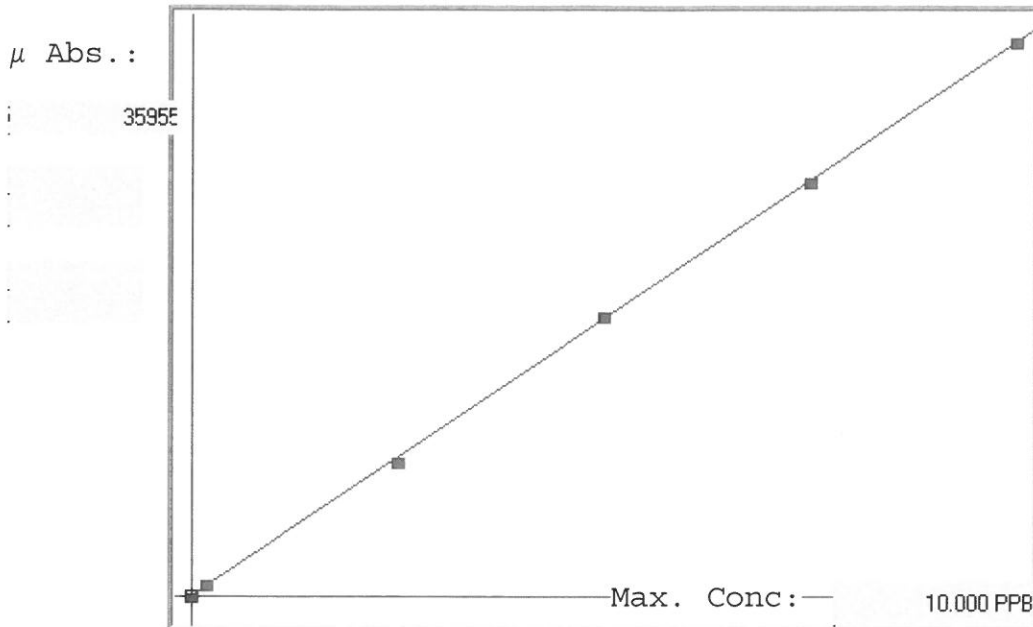

A= 0.0000e+000

B= 2.7815e-004

C= -7.9245e-003

Rho= 0.9999441

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	79	0.000	79				
0.2	0.200	0.203	0.003	758	0.0 %	758				
2.5	2.500	2.438	-0.062	8795	0.0 %	8795				
5.0	5.000	5.069	0.069	18253	0.0 %	18253				
7.5	7.500	7.482	-0.018	26929	0.0 %	26929				
10.0	10.000	9.993	-0.007	35955	0.0 %	35955				

LB111762 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Oct 2020 11:55:30

Sample ID	Extended ID	μ Abs.	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	79	-	0.0007470A		PPB	30 Oct 2020 11:57:13	S	Std
0.2 - 1	50.2	758	-	0.20007470A		PPB	30 Oct 2020 11:59:30	S	Std
2.5 - 1	52.5	8795	-	2.50007470A		PPB	30 Oct 2020 12:01:47	S	Std
5.0 - 1	55	18253	-	5.00007470A		PPB	30 Oct 2020 12:04:04	S	Std
7.5 - 1	57.5	26929	-	7.50007470A		PPB	30 Oct 2020 12:06:20	S	Std
10.0 - 1	59	35955	-	10.00007470A		PPB	30 Oct 2020 12:08:36	S	Std
ICV81 - 1	ICV81	13161	3.6528	-7470A		PPB	30 Oct 2020 12:11:15	U	SMPL
ICB81 - 1	ICB81	-89	-0.0327	-7470A		PPB	30 Oct 2020 12:13:30	U	SMPL
CCV39 - 1	CCV39	17993	4.9969	-7470A		PPB	30 Oct 2020 12:15:45	U	SMPL
CCB39 - 1	CCB39	-82	-0.0307	-7470A		PPB	30 Oct 2020 12:18:00	U	SMPL
CRA - 1	CRA	718	0.1918	-7470A		PPB	30 Oct 2020 12:20:14	U	SMPL
HighStd - 1	HighStd	35949	9.9913	-7470A		PPB	30 Oct 2020 12:22:29	U	SMPL
ChkStd - 1	ChkStd	25356	7.0449	-7470A		PPB	30 Oct 2020 12:24:45	U	SMPL
PB132729BL - 1	PBW	-181	-0.0583	-7470A		PPB	30 Oct 2020 12:27:01	U	SMPL
PB132729BS - 1	LCSW	14260	3.9585	-7470A		PPB	30 Oct 2020 12:29:17	U	SMPL
L4215-04 - 1	AU-05-102820	-82	-0.0307	-7470A		PPB	30 Oct 2020 12:31:34	U	SMPL
L4217-11 - 1	HR-01-102820	-2	-0.0085	-7470A		PPB	30 Oct 2020 12:33:50	U	SMPL
L4227-10 - 1	BU-02-102820	-19	-0.0132	-7470A		PPB	30 Oct 2020 12:36:07	U	SMPL
L4531-05 - 1	COMP-A-B-C	2	-0.0074	-7470A		PPB	30 Oct 2020 12:38:24	U	SMPL
L4531-05DUP - 1	COMP-A-B-CDUP	5	-0.0065	-7470A		PPB	30 Oct 2020 12:40:39	U	SMPL
CCV40 - 1	CCV40	17816	4.9476	-7470A		PPB	30 Oct 2020 12:42:54	U	SMPL
CCB40 - 1	CCB40	-81	-0.0305	-7470A		PPB	30 Oct 2020 12:45:09	U	SMPL
L4531-05MS - 1	COMP-A-B-CMS	14331	3.9783	-7470A		PPB	30 Oct 2020 12:47:24	U	SMPL
L4531-05MSD - 1	COMP-A-B-CMSD	14736	4.0909	-7470A		PPB	30 Oct 2020 12:49:40	U	SMPL
L4549-01 - 1	BUS-WASH-RECLAMATION-PIT	261	0.0647	-7470A		PPB	30 Oct 2020 12:51:55	U	SMPL
L4549-02 - 1	CHASSIS-WASH	-12	-0.0113	-7470A		PPB	30 Oct 2020 12:54:11	U	SMPL
PB132729TB - 1	PB132687TB	-11	-0.0110	-7470A		PPB	30 Oct 2020 12:56:26	U	SMPL
L4531-05LX5 - 1		2	-0.0074	-7470A		PPB	30 Oct 2020 12:58:43	U	SMPL
L4531-05A - 1		14434	4.0069	-7470A		PPB	30 Oct 2020 13:00:59	U	SMPL
CCV41 - 1	CCV41	18204	5.0555	-7470A		PPB	30 Oct 2020 13:03:16	U	SMPL
CCB41 - 1	CCB41	-85	-0.0316	-7470A		PPB	30 Oct 2020 13:05:33	U	SMPL