


LB111774

7470A

INSTRUMENT ID: CV1

Linear

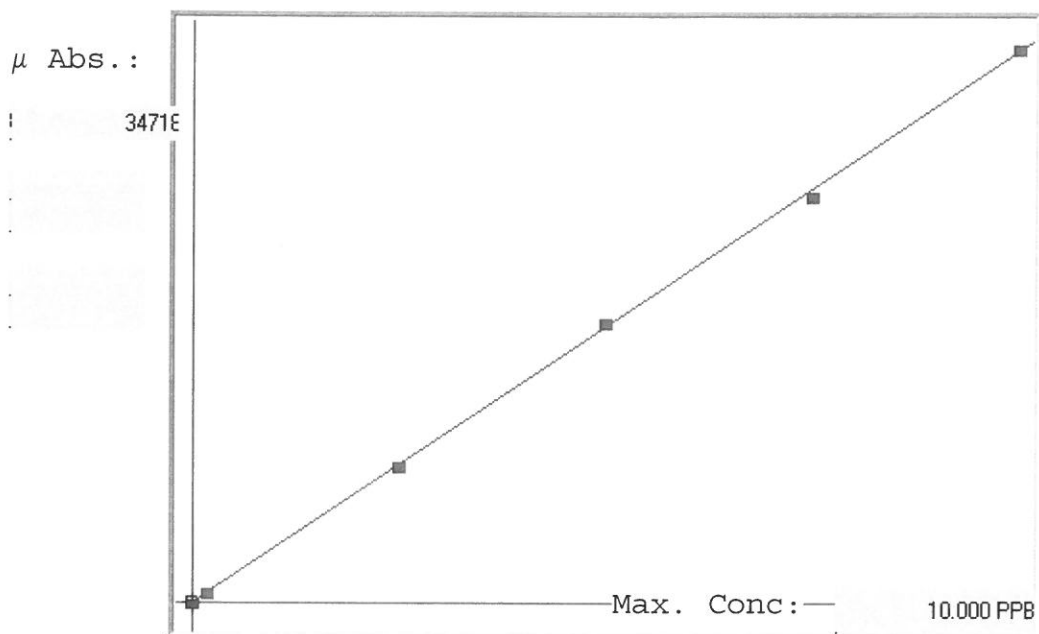

A= 0.0000e+000

B= 2.8919e-004

C= 4.3738e-005

Rho= 0.9998882

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.016	0.016	55	0.000	55				
0.2	0.200	0.183	-0.017	631	0.0 %	631				
2.5	2.500	2.488	-0.012	8602	0.0 %	8602				
5.0	5.000	5.075	0.075	17550	0.0 %	17550				
7.5	7.500	7.399	-0.101	25584	0.0 %	25584				
10.0	10.000	10.040	0.040	34718	0.0 %	34718				

LB111774 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Oct 2020 15:41:10

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SC	55	-	0.0000	7470A	PPB	30 Oct 2020 15:42:21	S	Std
0.2 - 1	SC-2	631	-	0.2000	7470A	PPB	30 Oct 2020 15:44:38	S	Std
2.5 - 1	SC-5	8602	-	2.5000	7470A	PPB	30 Oct 2020 15:46:55	S	Std
5.0 - 1	SC-5	17550	-	5.0000	7470A	PPB	30 Oct 2020 15:49:12	S	Std
7.5 - 1	SC-5	25584	-	7.5000	7470A	PPB	30 Oct 2020 15:54:11	S	Std
10.0 - 1	SC-10	34718	-	10.0000	7470A	PPB	30 Oct 2020 15:59:10	S	Std
ICV82 - 1	ICV82	13799	3.9905	-	7470A	PPB	30 Oct 2020 16:01:48	U	SMPL
ICB82 - 1	ICB82	-95	-0.0274	-	7470A	PPB	30 Oct 2020 16:04:03	U	SMPL
CCV44 - 1	CCV44	17682	5.1134	-	7470A	PPB	30 Oct 2020 16:06:17	U	SMPL
CCB44 - 1	CCB44	-104	-0.0300	-	7470A	PPB	30 Oct 2020 16:08:32	U	SMPL
CRA - 1	CRA	583	0.1686	-	7470A	PPB	30 Oct 2020 16:10:47	U	SMPL
HighStd - 1	HighStd	35451	10.2520	-	7470A	PPB	30 Oct 2020 16:13:02	U	SMPL
ChkStd - 1	ChkStd	24856	7.1881	-	7470A	PPB	30 Oct 2020 16:15:17	U	SMPL
PB132754BL - 1	PBW	-143	-0.0413	-	7470A	PPB	30 Oct 2020 16:17:33	U	SMPL
PB132754BS - 1	LCSW	11933	3.4509	-	7470A	PPB	30 Oct 2020 16:19:49	U	SMPL
L4222-11 - 1	EO-02-102920	-10	-0.0028	-	7470A	PPB	30 Oct 2020 16:22:05	U	SMPL
L4222-11DUP - 1	EO-02-102920DUP	35	0.0102	-	7470A	PPB	30 Oct 2020 16:24:22	U	SMPL
L4222-11MS - 1	EO-02-102920MS	11684	3.3789	-	7470A	PPB	30 Oct 2020 16:26:38	U	SMPL
L4222-11MSD - 1	EO-02-102920MSD	12595	3.6424	-	7470A	PPB	30 Oct 2020 16:34:26	U	SMPL
L4488-08 - 1	202	-31	-0.0089	-	7470A	PPB	30 Oct 2020 16:36:40	U	SMPL
CCV45 - 1	CCV45	18004	5.2066	-	7470A	PPB	30 Oct 2020 16:38:55	U	SMPL
CCB45 - 1	CCB45	-95	-0.0274	-	7470A	PPB	30 Oct 2020 16:41:10	U	SMPL
L4568-01 - 1	CHASSIS-WASH	41	0.0119	-	7470A	PPB	30 Oct 2020 16:43:26	U	SMPL
L4568-02 - 1	RECLAMATION-PIT	227	0.0657	-	7470A	PPB	30 Oct 2020 16:45:40	U	SMPL
PB132755BL - 1	PBW	-17	-0.0049	-	7470A	PPB	30 Oct 2020 16:47:56	U	SMPL
PB132755BS - 1	LCSW	12180	3.5223	-	7470A	PPB	30 Oct 2020 16:50:12	U	SMPL
L4434-11 - 1	40978-A	274	0.0793	-	7470A	PPB	30 Oct 2020 16:52:28	U	SMPL
L4434-11DUP - 1	40978-ADUP	236	0.0683	-	7470A	PPB	30 Oct 2020 16:57:56	U	SMPL
L4434-11MS - 1	40978-AMS	14673	4.2433	-	7470A	PPB	30 Oct 2020 17:00:12	U	SMPL
L4434-11MSD - 1	40978-AMSD	14818	4.2852	-	7470A	PPB	30 Oct 2020 17:02:29	U	SMPL
PB132756BL - 1	PBW	-77	-0.0222	-	7470A	PPB	30 Oct 2020 17:04:45	U	SMPL
PB132756BS - 1	LCSW	12567	3.6343	-	7470A	PPB	30 Oct 2020 17:07:01	U	SMPL
CCV46 - 1	CCV46	17785	5.1432	-	7470A	PPB	30 Oct 2020 17:09:16	U	SMPL
CCB46 - 1	CCB46	-65	-0.0188	-	7470A	PPB	30 Oct 2020 17:11:32	U	SMPL
L4576-01 - 1	PW-1	-27	-0.0078	-	7470A	PPB	30 Oct 2020 17:13:47	U	SMPL
L4576-01DUP - 1	PW-1DUP	0	0.0000	-	7470A	PPB	30 Oct 2020 17:16:03	U	SMPL
L4576-01MS - 1	PW-1MS	13240	3.8289	-	7470A	PPB	30 Oct 2020 17:18:18	U	SMPL
L4576-01MSD - 1	PW-1MSD	12682	3.6675	-	7470A	PPB	30 Oct 2020 17:20:34	U	SMPL
L4576-02 - 1	PW-2	-66	-0.0190	-	7470A	PPB	30 Oct 2020 17:22:50	U	SMPL
PB132754TB - 1	PB132724TB	15	0.0044	-	7470A	PPB	30 Oct 2020 17:25:06	U	SMPL
PB132755TB - 1	PB132738TB	8	0.0024	-	7470A	PPB	30 Oct 2020 17:27:23	U	SMPL
CCV47 - 1	CCV47	17951	5.1912	-	7470A	PPB	30 Oct 2020 17:29:40	U	SMPL
CCB47 - 1	CCB47	-84	-0.0242	-	7470A	PPB	30 Oct 2020 17:31:57	U	SMPL
L4222-11LX5 - 1		29	0.0084	-	7470A	PPB	30 Oct 2020 17:34:13	U	SMPL
L4222-11A - 1		14587	4.2184	-	7470A	PPB	30 Oct 2020 17:36:28	U	SMPL
L4434-11LX5 - 1		-36	-0.0104	-	7470A	PPB	30 Oct 2020 17:38:44	U	SMPL
L4434-11A - 1		14681	4.2456	-	7470A	PPB	30 Oct 2020 17:40:59	U	SMPL
L4576-01LX5 - 1		-89	-0.0257	-	7470A	PPB	30 Oct 2020 17:43:15	U	SMPL
L4576-01A - 1		13392	3.8728	-	7470A	PPB	30 Oct 2020 17:49:39	U	SMPL
CCV48 - 1	CCV48	17671	5.1103	-	7470A	PPB	30 Oct 2020 17:51:54	U	SMPL
CCB48 - 1	CCB48	-92	-0.0266	-	7470A	PPB	30 Oct 2020 17:54:10	U	SMPL