


LB 111823

ISM02.4

INSTRUMENT ID : CV1

 μ Abs. :

42309

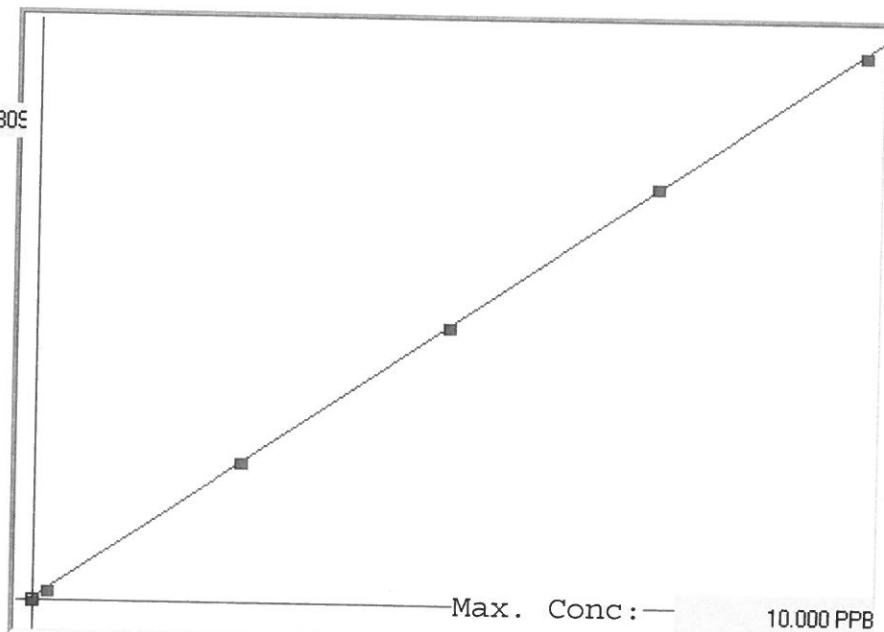

Linear

A= 0.0000e+000

B= 2.3586e-004

C= -2.2166e-002

Rho= 0.9999624

Accept = Accepted

slope
y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.006	-0.006	68	0.000	68					
0.05	0.050					400					
0.20	0.200	0.173	-0.027	827	0.0 %	827					
2.50	2.500	2.530	0.030	10823	0.0 %	10823					
5.00	5.000	4.996	-0.004	21275	0.0 %	21275					
7.50	7.500	7.550	0.050	32107	0.0 %	32107					
10.0	10.000	9.957	-0.043	42309	0.0 %	42309					

14
=

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	68	-		0 ISM02.4	PPB	11/4/2020 11:27	Std
	0.2 S0.2	827	-		0.2 ISM02.4	PPB	11/4/2020 11:29	Std
	2.5 S2.5	10823	-		2.5 ISM02.4	PPB	11/4/2020 11:31	Std
	5 S5.0	21275	-		5 ISM02.4	PPB	11/4/2020 11:33	Std
	7.5 S7.5	32107	-		7.5 ISM02.4	PPB	11/4/2020 11:36	Std
	10 S10.0	42309	-		10 ISM02.4	PPB	11/4/2020 11:38	Std
ICV	ICV	16449	3.8574 -		ISM02.4	PPB	11/4/2020 11:41	SMPL
ICB	ICB	6	-0.0208 -		ISM02.4	PPB	11/4/2020 11:43	SMPL
CCV066	CCV066	21835	5.1277 -		ISM02.4	PPB	11/4/2020 11:45	SMPL
CCB066	CCB066	-29	-0.029 -		ISM02.4	PPB	11/4/2020 11:48	SMPL
PB132811BL	PBS811	39	-0.013 -		ISM02.4	PPB	11/4/2020 11:50	SMPL
L4581-01	ME4511	1904	0.4269 -		ISM02.4	PPB	11/4/2020 11:52	SMPL
L4581-02	ME4512	1156	0.2505 -		ISM02.4	PPB	11/4/2020 11:54	SMPL
L4581-03	ME4514	1086	0.234 -		ISM02.4	PPB	11/4/2020 11:57	SMPL
L4581-04	ME4521	1421	0.313 -		ISM02.4	PPB	11/4/2020 11:59	SMPL
L4581-05	ME4522	2411	0.5465 -		ISM02.4	PPB	11/4/2020 12:01	SMPL
L4581-06	ME4530	236	0.0335 -		ISM02.4	PPB	11/4/2020 12:03	SMPL
L4581-07	ME4531	261	0.0394 -		ISM02.4	PPB	11/4/2020 12:06	SMPL
L4581-08	ME4532	315	0.0521 -		ISM02.4	PPB	11/4/2020 12:08	SMPL
L4581-09	ME4533	213	0.0281 -		ISM02.4	PPB	11/4/2020 12:10	SMPL
L4581-10	ME4533D	198	0.0245 -		ISM02.4	PPB	11/4/2020 12:12	SMPL
L4581-11	ME4533S	10820	2.5298 -		ISM02.4	PPB	11/4/2020 12:15	SMPL
L4581-18	ME4527	125	0.0073 -		ISM02.4	PPB	11/4/2020 12:17	SMPL
L4581-19	ME4528	183	0.021 -		ISM02.4	PPB	11/4/2020 12:19	SMPL
L4581-20	ME4529	126	0.0076 -		ISM02.4	PPB	11/4/2020 12:21	SMPL
PB132812BL	PBS812	24	-0.0165 -		ISM02.4	PPB	11/4/2020 12:24	SMPL
L4582-01	ME4503	1136	0.2458 -		ISM02.4	PPB	11/4/2020 12:26	SMPL
L4582-02	ME4504	900	0.1901 -		ISM02.4	PPB	11/4/2020 12:28	SMPL
L4582-03	ME4505	1052	0.226 -		ISM02.4	PPB	11/4/2020 12:31	SMPL
L4582-04	ME4506	727	0.1493 -		ISM02.4	PPB	11/4/2020 12:33	SMPL
CCV067	CCV067	21837	5.1282 -		ISM02.4	PPB	11/4/2020 12:35	SMPL
CCB067	CCB067	-10	-0.0245 -		ISM02.4	PPB	11/4/2020 12:37	SMPL
L4582-05	ME4507	808	0.1684 -		ISM02.4	PPB	11/4/2020 12:40	SMPL
L4582-06	ME4508	742	0.1528 -		ISM02.4	PPB	11/4/2020 12:42	SMPL
L4582-07	ME4508D	739	0.1521 -		ISM02.4	PPB	11/4/2020 12:44	SMPL
L4582-08	ME4508S	10899	2.5484 -		ISM02.4	PPB	11/4/2020 12:46	SMPL
L4582-09	ME4509	1184	0.2571 -		ISM02.4	PPB	11/4/2020 12:49	SMPL
L4582-10	ME4510	1019	0.2182 -		ISM02.4	PPB	11/4/2020 12:51	SMPL
L4582-11	ME4513	859	0.1804 -		ISM02.4	PPB	11/4/2020 12:53	SMPL
L4582-12	ME4515	680	0.1382 -		ISM02.4	PPB	11/4/2020 12:55	SMPL
L4582-13	ME4516	993	0.212 -		ISM02.4	PPB	11/4/2020 12:58	SMPL
L4582-14	ME4517	893	0.1885 -		ISM02.4	PPB	11/4/2020 13:00	SMPL
L4582-15	ME4518	1160	0.2514 -		ISM02.4	PPB	11/4/2020 13:02	SMPL
L4582-16	ME4519	1156	0.2505 -		ISM02.4	PPB	11/4/2020 13:05	SMPL
L4582-17	ME4520	1414	0.3113 -		ISM02.4	PPB	11/4/2020 13:07	SMPL
L4582-18	ME4523	130	0.0085 -		ISM02.4	PPB	11/4/2020 13:09	SMPL

LB111823

INSTRUMENT ID : CV1

L4582-19	ME4524	169	0.0177 -	ISM02.4	PPB	11/4/2020 13:11 SMPL
L4582-20	ME4525	185	0.0215 -	ISM02.4	PPB	11/4/2020 13:14 SMPL
L4582-21	ME4526	177	0.0196 -	ISM02.4	PPB	11/4/2020 13:16 SMPL
CCV068	CCV068	21744	5.1063 -	ISM02.4	PPB	11/4/2020 13:18 SMPL
CCB068	CCB068	-3	-0.0229 -	ISM02.4	PPB	11/4/2020 13:20 SMPL
PB132813BL	PBS813	36	-0.0137 -	ISM02.4	PPB	11/4/2020 13:23 SMPL
L4556-19	MX2Q05	9576	2.2364 -	ISM02.4	PPB	11/4/2020 13:27 SMPL
L4556-20	MX2Q05D	9091	2.122 -	ISM02.4	PPB	11/4/2020 13:32 SMPL
L4556-21	MX2Q05S	19662	4.6152 -	ISM02.4	PPB	11/4/2020 13:34 SMPL
CCV069	CCV069	21897	5.1424 -	ISM02.4	PPB	11/4/2020 13:41 SMPL
CCB069	CCB069	-12	-0.025 -	ISM02.4	PPB	11/4/2020 13:44 SMPL