


LB111844

7470A

INSTRUMENT ID: CV4

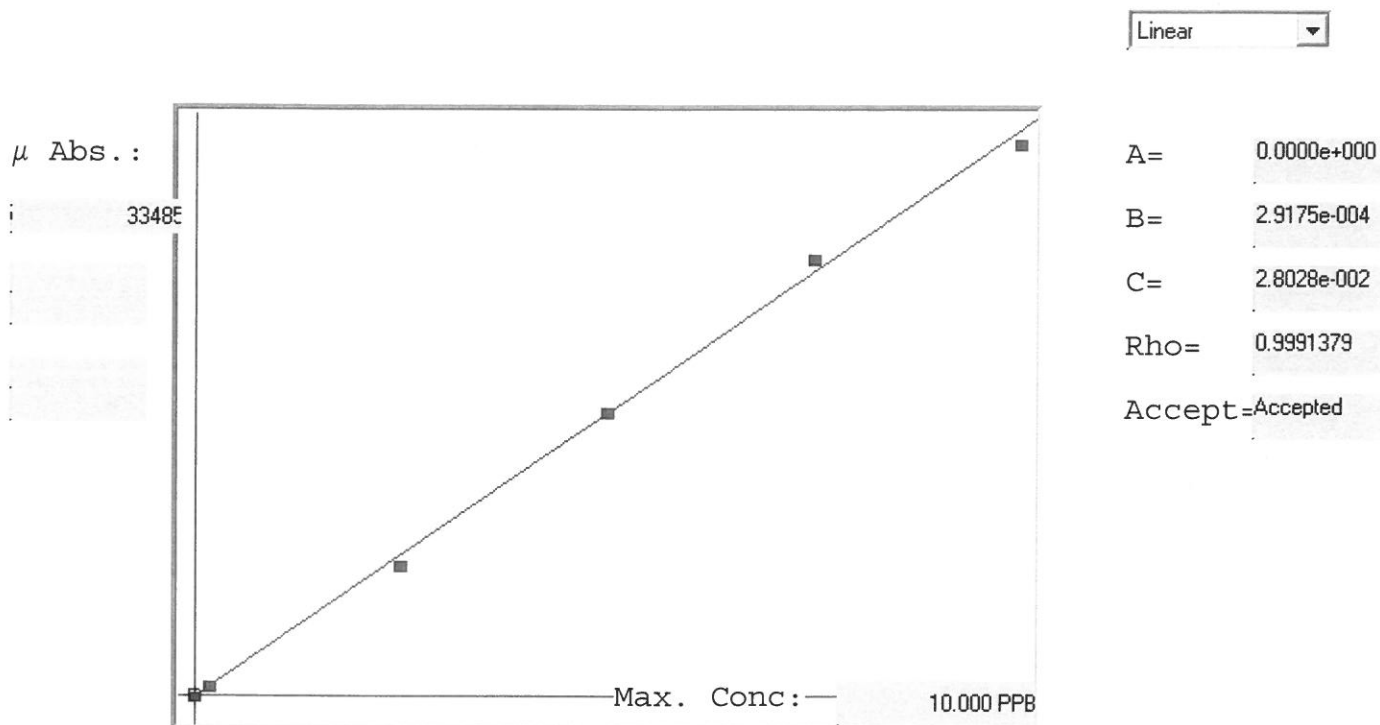

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.027	0.027	-4	0.000	-4				
0.2	0.200	0.211	0.011	626	0.0 %	626				
2.5	2.500	2.342	-0.158	7930	0.0 %	7930				
5.0	5.000	5.059	0.059	17243	0.0 %	17243				
7.5	7.500	7.765	0.265	26520	0.0 %	26520				
10.0	10.000	9.797	-0.203	33485	0.0 %	33485				

LB111844 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 05 Nov 2020 09:58:39				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-4	-	0.00007470A	PPB	05 Nov 2020 09:59:51	S	Std
0.2 - 1	50.2	626	-	0.20007470A	PPB	05 Nov 2020 10:02:08	S	Std
2.5 - 1	52.5	7930	-	2.50007470A	PPB	05 Nov 2020 10:04:26	S	Std
5.0 - 1	55	17243	-	5.00007470A	PPB	05 Nov 2020 10:06:43	S	Std
7.5 - 1	57.5	26520	-	7.50007470A	PPB	05 Nov 2020 10:08:59	S	Std
10.0 - 1	510	33485	-	10.00007470A	PPB	05 Nov 2020 10:11:15	S	Std
ICV89 - 1	ICV89	12296	3.6153	-7470A	PPB	05 Nov 2020 10:14:00	U	SMPL
ICB89 - 1	ICB89	-102	-0.0017	-7470A	PPB	05 Nov 2020 10:16:15	U	SMPL
CCV74 - 1	CCV74	16624	4.8780	-7470A	PPB	05 Nov 2020 10:18:30	U	SMPL
CCB74 - 1	CCB74	-107	-0.0032	-7470A	PPB	05 Nov 2020 10:20:45	U	SMPL
CRA - 1	CRA	574	0.1955	-7470A	PPB	05 Nov 2020 10:23:00	U	SMPL
HighStd - 1	HighStd	32465	9.4996	-7470A	PPB	05 Nov 2020 10:25:14	U	SMPL
ChkStd - 1	ChkStd	21777	6.3814	-7470A	PPB	05 Nov 2020 10:27:29	U	SMPL
PB132827BL - 1	PBW	-144	-0.0140	-7470A	PPB	05 Nov 2020 10:29:46	U	SMPL
PB132827BS - 1	LCSW	12195	3.5859	-7470A	PPB	05 Nov 2020 10:32:02	U	SMPL
L4621-04 - 1	PAV-B8-110320-0-10	-76	0.0059	-7470A	PPB	05 Nov 2020 10:34:18	U	SMPL
L4621-04DUP - 1	PAV-B8-110320-0-10DUP	-9	0.0254	-7470A	PPB	05 Nov 2020 10:36:35	U	SMPL
L4621-04MS - 1	PAV-B8-110320-0-10MS	12541	3.6868	-7470A	PPB	05 Nov 2020 10:38:52	U	SMPL
L4621-04MSD - 1	PAV-B8-110320-0-10MSD	12674	3.7256	-7470A	PPB	05 Nov 2020 10:41:09	U	SMPL
L4621-06 - 1	PAV-B8-110320-10-20	-79	0.0050	-7470A	PPB	05 Nov 2020 10:43:24	U	SMPL
CCV75 - 1	CCV75	16751	4.9151	-7470A	PPB	05 Nov 2020 10:45:40	U	SMPL
CCB75 - 1	CCB75	-95	0.0003	-7470A	PPB	05 Nov 2020 10:47:55	U	SMPL
PB132828BL - 1	PBW	-5	0.0266	-7470A	PPB	05 Nov 2020 10:50:11	U	SMPL
PB132828BS - 1	LCSW	12198	3.5867	-7470A	PPB	05 Nov 2020 10:52:26	U	SMPL
L4612-01 - 1	265316	236	0.0969	-7470A	PPB	05 Nov 2020 10:54:41	U	SMPL
L4612-01DUP - 1	265316DUP	200	0.0864	-7470A	PPB	05 Nov 2020 10:56:57	U	SMPL
L4612-01MS - 1	265316MS	11985	3.5246	-7470A	PPB	05 Nov 2020 10:59:13	U	SMPL
L4612-01MSD - 1	265316MSD	11378	3.3475	-7470A	PPB	05 Nov 2020 11:04:03	U	SMPL
L4621-09 - 1	FIELD-BLANK	-151	-0.0160	-7470A	PPB	05 Nov 2020 11:06:19	U	SMPL
CCV76 - 1	CCV76	16130	4.7339	-7470A	PPB	05 Nov 2020 11:08:37	U	SMPL
CCB76 - 1	CCB76	-89	0.0021	-7470A	PPB	05 Nov 2020 11:10:54	U	SMPL
PB132827TB - 1	PB132809TB	-11	0.0248	-7470A	PPB	05 Nov 2020 11:13:09	U	SMPL
L4621-04LX5 - 1		0	0.0280	-7470A	PPB	05 Nov 2020 11:15:25	U	SMPL
L4621-04A - 1		13850	4.0687	-7470A	PPB	05 Nov 2020 11:17:40	U	SMPL
L4612-01LX5 - 1		-74	0.0064	-7470A	PPB	05 Nov 2020 11:19:56	U	SMPL
L4612-01A - 1		15912	4.6703	-7470A	PPB	05 Nov 2020 11:22:12	U	SMPL
CCV77 - 1	CCV77	17143	5.0294	-7470A	PPB	05 Nov 2020 11:24:28	U	SMPL
CCB77 - 1	CCB77	-111	-0.0044	-7470A	PPB	05 Nov 2020 11:26:44	U	SMPL