


LB111867

ISM02.4

INSTRUMENT ID: CV4

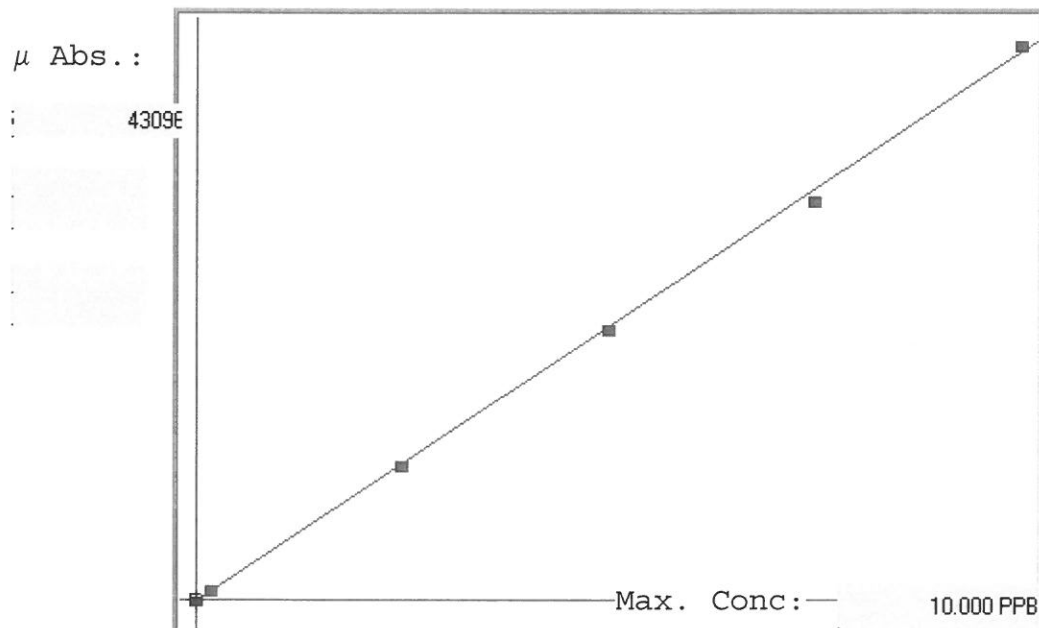

Linear

A= 0.0000e+000

B= 2.3415e-004

C= 3.7280e-002

Rho= 0.9997117

Accept=Accepted

stope
y=mx+intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.048	0.048	47	0.000	47					-
0.05	0.050					400					-
0.20	0.200	0.214	0.014	755	0.0 %	755					-
2.50	2.500	2.485	-0.015	10455	0.0 %	10455					-1
5.00	5.000	4.991	-0.009	21154	0.0 %	21154					0
7.50	7.500	7.333	-0.167	31159	0.0 %	31159					-2
10.0	10.000	10.128	0.128	43096	0.0 %	43096					1

LB111867
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	47	-		0 ISM02.4	PPB	11/6/2020 12:30	Std
	0.2 S0.2	755	-		0.2 ISM02.4	PPB	11/6/2020 12:33	Std
	2.5 S2.5	10455	-		2.5 ISM02.4	PPB	11/6/2020 12:35	Std
	5 S5.0	21154	-		5 ISM02.4	PPB	11/6/2020 12:37	Std
	7.5 S7.5	31159	-		7.5 ISM02.4	PPB	11/6/2020 12:39	Std
	10 S10.0	43096	-		10 ISM02.4	PPB	11/6/2020 12:44	Std
ICV	ICV	16716	3.9514 -		ISM02.4	PPB	11/6/2020 12:47	SMPL
ICB	ICB	-86	0.0171 -		ISM02.4	PPB	11/6/2020 12:49	SMPL
CCV086	CCV086	21318	5.029 -		ISM02.4	PPB	11/6/2020 12:51	SMPL
CCB086	CCB086	-76	0.0195 -		ISM02.4	PPB	11/6/2020 12:54	SMPL
L4626-01	MEW0T4	1035	0.2796 -		ISM02.4	PPB	11/6/2020 13:01	SMPL
L4626-02	MEW0T5	805	0.2258 -		ISM02.4	PPB	11/6/2020 13:03	SMPL
L4626-03	MEW0T7	682	0.197 -		ISM02.4	PPB	11/6/2020 13:05	SMPL
L4626-04	MEW0T7D	657	0.1911 -		ISM02.4	PPB	11/6/2020 13:07	SMPL
L4626-05	MEW0T7S	4506	1.0924 -		ISM02.4	PPB	11/6/2020 13:10	SMPL
PB132867BL	PBW867	17	0.0413 -		ISM02.4	PPB	11/6/2020 13:12	SMPL
CCV087	CCV087	21157	4.9913 -		ISM02.4	PPB	11/6/2020 13:14	SMPL
CCB087	CCB087	-51	0.0253 -		ISM02.4	PPB	11/6/2020 13:17	SMPL