


LB111883

7470A

INSTRUMENT ID: CV1

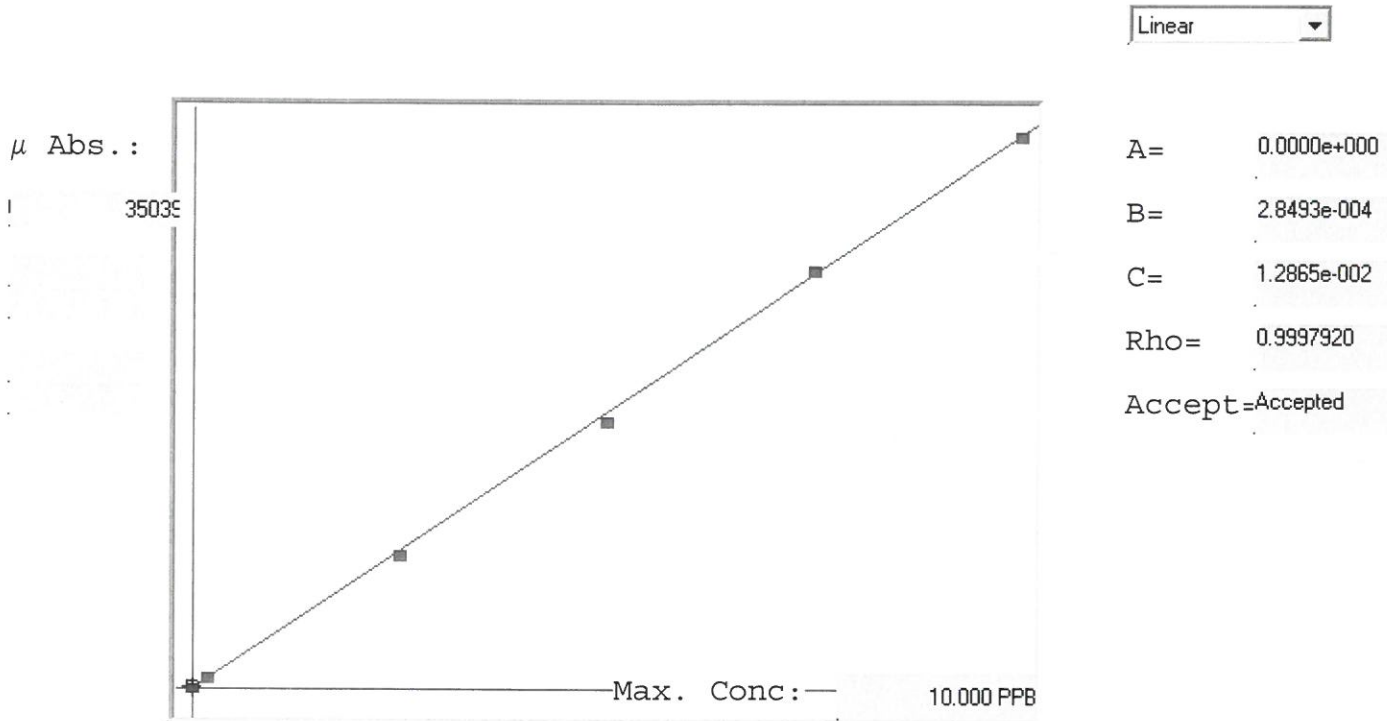

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.050	0.050	129	0.000	129				
0.2	0.200	0.238	0.038	791	0.0 %	791				
2.5	2.500	2.437	-0.063	8508	0.0 %	8508				
5.0	5.000	4.876	-0.124	17066	0.0 %	17066				
7.5	7.500	7.603	0.103	26638	0.0 %	26638				
10.0	10.000	9.997	-0.003	35039	0.0 %	35039				

LB111883 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 09 Nov 2020 09:43:04					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	129	-	0.0000	7470A	PPB	09 Nov 2020 09:47:51	S	Std
0.2 - 1	50.2	791	-	0.2000	7470A	PPB	09 Nov 2020 09:50:08	S	Std
2.5 - 1	52.5	8508	-	2.5000	7470A	PPB	09 Nov 2020 09:52:25	S	Std
5.0 - 1	55	17066	-	5.0000	7470A	PPB	09 Nov 2020 09:54:42	S	Std
7.5 - 1	57.5	26638	-	7.5000	7470A	PPB	09 Nov 2020 09:56:58	S	Std
10.0 - 1	518	35039	-	10.0000	7470A	PPB	09 Nov 2020 09:59:14	S	Std
ICV93 - 1	ICV93	14239	4.0700	-	7470A	PPB	09 Nov 2020 10:02:16	U	SMPL
ICB93 - 1	ICB93	26	0.0203	-	7470A	PPB	09 Nov 2020 10:04:31	U	SMPL
CCV93 - 1	CCV93	15894	4.5416	-	7470A	PPB	09 Nov 2020 10:06:46	U	SMPL
CCB93 - 1	CCB93	2	0.0134	-	7470A	PPB	09 Nov 2020 10:09:01	U	SMPL
CRA - 1	CRA	784	0.2363	-	7470A	PPB	09 Nov 2020 10:11:16	U	SMPL
HighStd - 1	HighStd	34623	9.8781	-	7470A	PPB	09 Nov 2020 10:13:31	U	SMPL
ChkStd - 1	ChkStd	24839	7.0903	-	7470A	PPB	09 Nov 2020 10:15:46	U	SMPL
PB132884BL - 1	PBW	-24	0.0060	-	7470A	PPB	09 Nov 2020 10:18:03	U	SMPL
PB132884BS - 1	LCSW	12686	3.6275	-	7470A	PPB	09 Nov 2020 10:20:20	U	SMPL
L4637-01 - 1	TRE-1059	51	0.0274	-	7470A	PPB	09 Nov 2020 10:22:36	U	SMPL
L4651-01 - 1	PB-2020-WS-000-03	99	0.0411	-	7470A	PPB	09 Nov 2020 10:24:52	U	SMPL
L4656-02 - 1	SR-L14-L13-NORTH	133	0.0508	-	7470A	PPB	09 Nov 2020 10:27:09	U	SMPL
L4656-09 - 1	SR-L14-L13-SOUTH	154	0.0567	-	7470A	PPB	09 Nov 2020 10:29:26	U	SMPL
L4657-06 - 1	PAV-B49-110520-0-10	630	0.1924	-	7470A	PPB	09 Nov 2020 10:31:41	U	SMPL
CCV94 - 1	CCV94	17297	4.9413	-	7470A	PPB	09 Nov 2020 10:33:56	U	SMPL
CCB94 - 1	CCB94	45	0.0257	-	7470A	PPB	09 Nov 2020 10:36:12	U	SMPL
L4657-07 - 1	PAV-B49-110520-10-18	581	0.1784	-	7470A	PPB	09 Nov 2020 10:38:27	U	SMPL
L4657-07DUP - 1	PAV-B49-110520-10-18DUP	638	0.1947	-	7470A	PPB	09 Nov 2020 10:40:42	U	SMPL
L4657-07MS - 1	PAV-B49-110520-10-18MS	12967	3.7076	-	7470A	PPB	09 Nov 2020 10:42:58	U	SMPL
L4657-07MSD - 1	PAV-B49-110520-10-18MSD	14725	4.2085	-	7470A	PPB	09 Nov 2020 10:45:13	U	SMPL
PB132885BL - 1	PBW	63	0.0308	-	7470A	PPB	09 Nov 2020 10:47:29	U	SMPL
PB132885BS - 1	LCSW	12516	3.5791	-	7470A	PPB	09 Nov 2020 10:49:46	U	SMPL
L4636-09 - 1	DRUM-COMP-1-AU	699	0.2120	-	7470A	PPB	09 Nov 2020 10:57:01	U	SMPL
L4636-09DUP - 1	DRUM-COMP-1-AUDUP	599	0.1835	-	7470A	PPB	09 Nov 2020 10:59:18	U	SMPL
L4636-09MS - 1	DRUM-COMP-1-AUMS	12264	3.5073	-	7470A	PPB	09 Nov 2020 11:01:35	U	SMPL
L4636-09MSD - 1	DRUM-COMP-1-AUMSD	12835	3.6700	-	7470A	PPB	09 Nov 2020 11:06:57	U	SMPL
CCV95 - 1	CCV95	16948	4.8419	-	7470A	PPB	09 Nov 2020 11:09:12	U	SMPL
CCB95 - 1	CCB95	79	0.0354	-	7470A	PPB	09 Nov 2020 11:11:27	U	SMPL
L4651-02 - 1	PS-2020-WW-000-03	123	0.0479	-	7470A	PPB	09 Nov 2020 11:13:43	U	SMPL
PB132884TB - 1	PB132854TB	142	0.0533	-	7470A	PPB	09 Nov 2020 11:15:58	U	SMPL
L4657-07LX5 - 1		235	0.0798	-	7470A	PPB	09 Nov 2020 11:18:13	U	SMPL
L4657-07A - 1		14184	4.0544	-	7470A	PPB	09 Nov 2020 11:20:29	U	SMPL
L4636-09LX5 - 1		404	0.1280	-	7470A	PPB	09 Nov 2020 11:22:45	U	SMPL
L4636-09A - 1		15696	4.4852	-	7470A	PPB	09 Nov 2020 11:25:02	U	SMPL
CCV96 - 1	CCV96	17096	4.8841	-	7470A	PPB	09 Nov 2020 11:27:19	U	SMPL
CCB96 - 1	CCB96	67	0.0320	-	7470A	PPB	09 Nov 2020 11:29:36	U	SMPL