


LB111903

7471B

INSTRUMENT ID: CV4

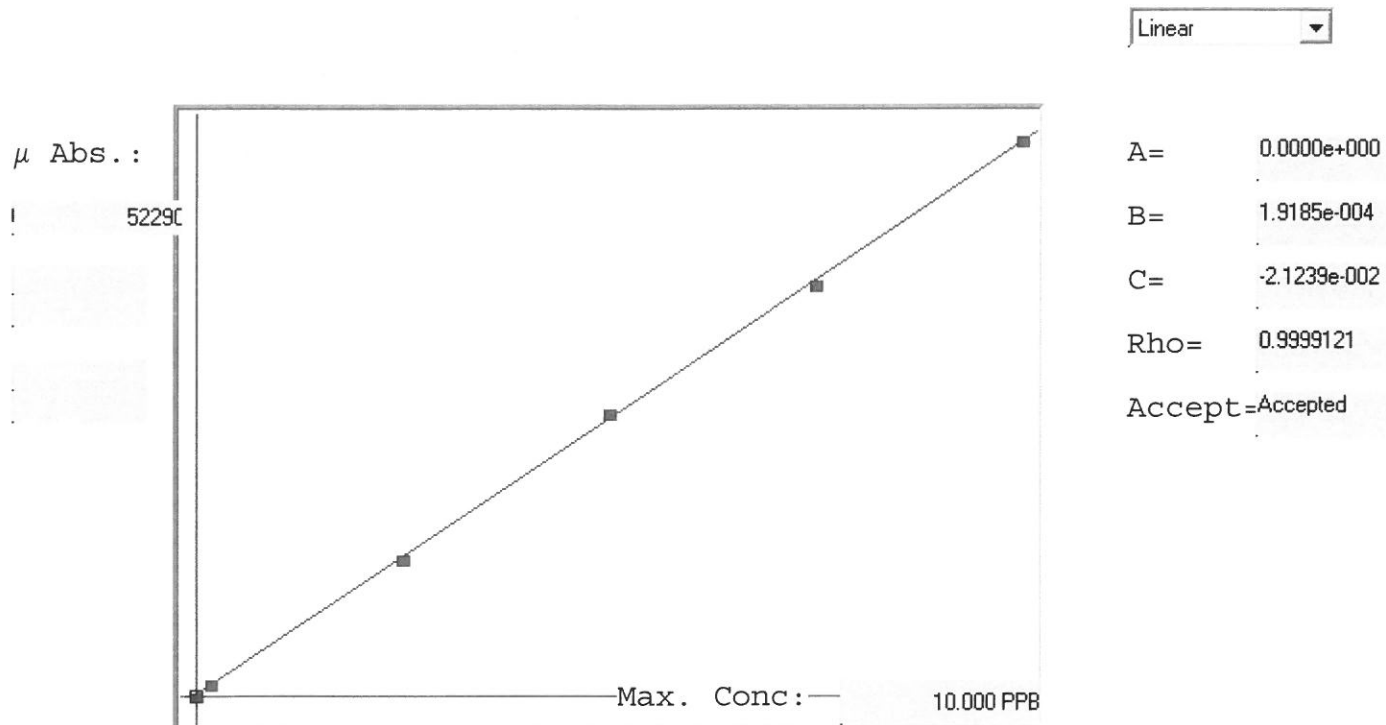

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.008	0.008	155	0.000	155				
0.2	0.200	0.198	-0.002	1141	0.0 %	1141				
2.5	2.500	2.453	-0.047	12899	0.0 %	12899				
5.0	5.000	5.091	0.091	26646	0.0 %	26646				
7.5	7.500	7.439	-0.061	38884	0.0 %	38884				
10.0	10.000	10.011	0.011	52290	0.0 %	52290				

LB111903 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 10 Nov 2020 14:35:49					
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type	
0.0 - 1	50	155	-	0.00007471B	PPB	10 Nov 2020 14:41:08	S	Std	
0.2 - 1	51.2	1141	-	0.20007471B	PPB	10 Nov 2020 14:43:25	S	Std	
2.5 - 1	52.1	12899	-	2.50007471B	PPB	10 Nov 2020 14:45:42	S	Std	
5.0 - 1	55	26646	-	5.00007471B	PPB	10 Nov 2020 14:47:59	S	Std	
7.5 - 1	57.5	38884	-	7.50007471B	PPB	10 Nov 2020 14:50:15	S	Std	
10.0 - 1	510	52290	-	10.00007471B	PPB	10 Nov 2020 14:52:32	S	Std	
ICV96 - 1	ICV96	20771	3.9637	-7471B	PPB	10 Nov 2020 14:55:16	U	SMPL	
ICB96 - 1	ICB96	10	-0.0193	-7471B	PPB	10 Nov 2020 14:57:31	U	SMPL	
CCV08 - 1	CCV08	26120	4.9900	-7471B	PPB	10 Nov 2020 14:59:46	U	SMPL	
CCB08 - 1	CCB08	13	-0.0187	-7471B	PPB	10 Nov 2020 15:02:00	U	SMPL	
CRA - 1	CRA	1006	0.1718	-7471B	PPB	10 Nov 2020 15:04:16	U	SMPL	
HighStd - 1	HighStd	51963	9.9480	-7471B	PPB	10 Nov 2020 15:06:31	U	SMPL	
ChkStd - 1	ChkStd	34287	6.5568	-7471B	PPB	10 Nov 2020 15:08:46	U	SMPL	
PB132917BL - 1	PBS	-122	-0.0446	-7471B	PPB	10 Nov 2020 15:11:03	U	SMPL	
PB132917BS - 1	LCSS	17449	3.3264	-7471B	PPB	10 Nov 2020 15:13:21	U	SMPL	
L4594-01 - 1	OR-03-110920	2471	0.4528	-7471B	PPB	10 Nov 2020 15:15:37	U	SMPL	
L4594-01DUP - 1	OR-03-110920DUP	2135	0.3884	-7471B	PPB	10 Nov 2020 15:17:53	U	SMPL	
L4594-01MS - 1	OR-03-110920MS	21917	4.1836	-7471B	PPB	10 Nov 2020 15:20:10	U	SMPL	
L4594-01MSD - 1	OR-03-110920MSD	20055	3.8264	-7471B	PPB	10 Nov 2020 15:22:27	U	SMPL	
L4656-01 - 1	SR-L14-L13-NORTH	20152	3.8450	-7471B	PPB	10 Nov 2020 15:24:42	U	SMPL	
CCV09 - 1	CCV09	26102	4.9865	-7471B	PPB	10 Nov 2020 15:26:57	U	SMPL	
CCB09 - 1	CCB09	-7	-0.0226	-7471B	PPB	10 Nov 2020 15:29:13	U	SMPL	
L4656-08 - 1	SR-L14-L13-SOUTH	21956	4.1911	-7471B	PPB	10 Nov 2020 15:31:28	U	SMPL	
L4679-01 - 1	FK-EF-03-001-ABCD	824	0.1368	-7471B	PPB	10 Nov 2020 15:33:43	U	SMPL	
L4680-01 - 1	PAV-B7-110520-0-10	29584	5.6545	-7471B	PPB	10 Nov 2020 15:35:59	U	SMPL	
L4680-03 - 1	PAV-B7-110520-DP	32878	6.2865	-7471B	PPB	10 Nov 2020 15:38:15	U	SMPL	
L4680-05 - 1	PAV-B7-110920-10-20	3114	0.5762	-7471B	PPB	10 Nov 2020 15:40:33	U	SMPL	
L4681-03 - 1	TP-1-S	1815	0.3270	-7471B	PPB	10 Nov 2020 15:42:50	U	SMPL	
L4681-07 - 1	TP-1-D	627	0.0991	-7471B	PPB	10 Nov 2020 15:45:07	U	SMPL	
L4594-01LX5 - 1		419	0.0591	-7471B	PPB	10 Nov 2020 15:47:24	U	SMPL	
L4594-01A - 1		21591	4.1211	-7471B	PPB	10 Nov 2020 15:49:40	U	SMPL	
CCV10 - 1	CCV10	25501	4.8712	-7471B	PPB	10 Nov 2020 15:51:56	U	SMPL	
CCB10 - 1	CCB10	43	-0.0130	-7471B	PPB	10 Nov 2020 15:54:12	U	SMPL	