


LB111939

7471B

INSTRUMENT ID: CV1

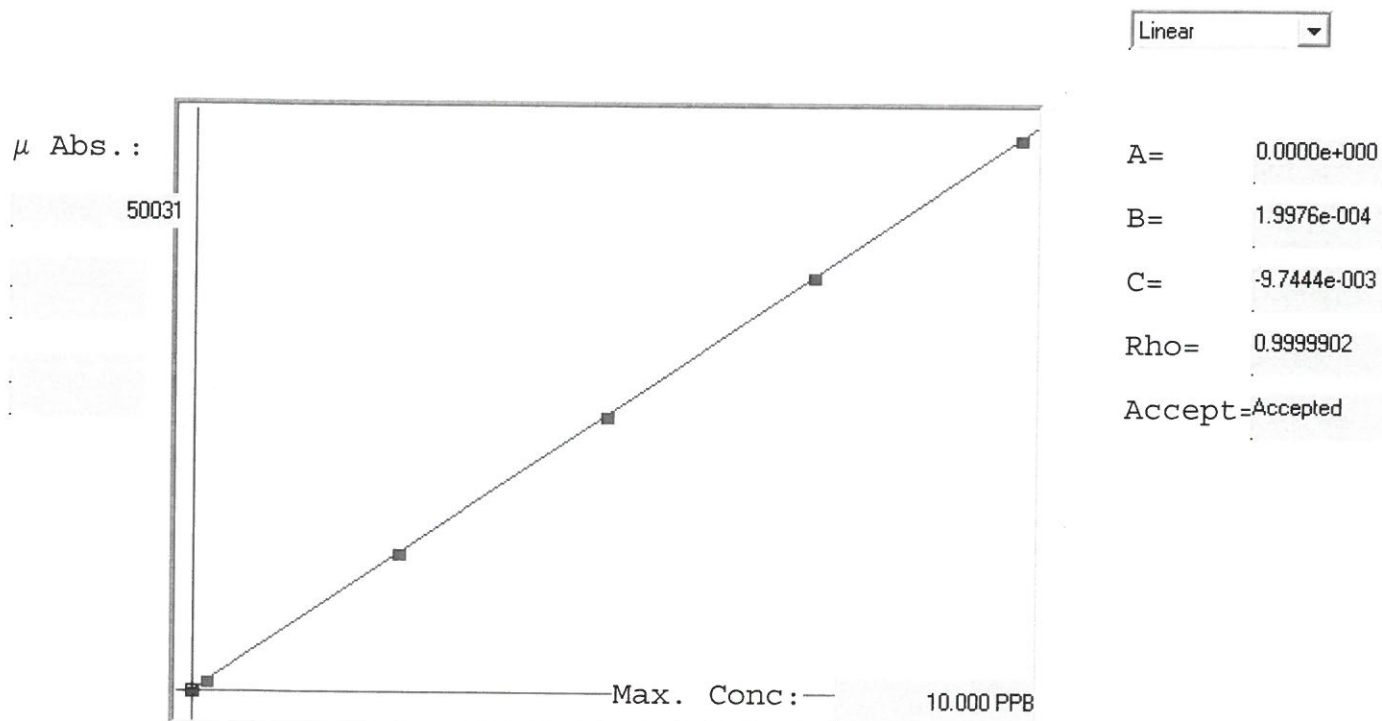

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.016	0.016	130	0.000	130				
0.2	0.200	0.175	-0.025	924	0.0 %	924				
2.5	2.500	2.506	0.006	12593	0.0 %	12593				
5.0	5.000	4.998	-0.002	25070	0.0 %	25070				
7.5	7.500	7.521	0.021	37697	0.0 %	37697				
10.0	10.000	9.984	-0.016	50031	0.0 %	50031				

LB111939 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 12 Nov 2020 13:25:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	130	-	0.00007471B	PPB		12 Nov 2020 13:28:17	S	Std
0.2 - 1	50.2	924	-	0.20007471B	PPB		12 Nov 2020 13:30:34	S	Std
2.5 - 1	52.5	12593	-	2.50007471B	PPB		12 Nov 2020 13:32:51	S	Std
5.0 - 1	55	25070	-	5.00007471B	PPB		12 Nov 2020 13:35:08	S	Std
7.5 - 1	57.5	37697	-	7.50007471B	PPB		12 Nov 2020 13:37:24	S	Std
10.0 - 1	50	50031	-	10.00007471B	PPB		12 Nov 2020 13:39:41	S	Std
ICV01 - 1	ICV01	19470	3.8796	-7471B	PPB		12 Nov 2020 13:42:22	U	SMPL
ICB01 - 1	ICB01	-14	-0.0125	-7471B	PPB		12 Nov 2020 13:44:37	U	SMPL
CCV20 - 1	CCV20	24515	4.8873	-7471B	PPB		12 Nov 2020 13:46:51	U	SMPL
CCB20 - 1	CCB20	-16	-0.0129	-7471B	PPB		12 Nov 2020 13:49:06	U	SMPL
CRA - 1	CRA	946	0.1792	-7471B	PPB		12 Nov 2020 13:51:22	U	SMPL
HighStd - 1	HighStd	48382	9.6550	-7471B	PPB		12 Nov 2020 13:53:37	U	SMPL
ChkStd - 1	ChkStd	34522	6.8863	-7471B	PPB		12 Nov 2020 13:58:38	U	SMPL
PB132959BL - 1	PBS	-88	-0.0273	-7471B	PPB		12 Nov 2020 14:00:53	U	SMPL
PB132959BS - 1	LCSS	18246	3.6350	-7471B	PPB		12 Nov 2020 14:03:11	U	SMPL
L4587-01 - 1	HR-02-111120	2737	0.5370	-7471B	PPB		12 Nov 2020 14:05:27	U	SMPL
L4587-01DUP - 1	HR-02-111120DUP	2585	0.5066	-7471B	PPB		12 Nov 2020 14:07:44	U	SMPL
L4587-01MS - 1	HR-02-111120MS	20116	4.0086	-7471B	PPB		12 Nov 2020 14:12:36	U	SMPL
L4587-01MSD - 1	HR-02-111120MSD	19571	3.8997	-7471B	PPB		12 Nov 2020 14:14:53	U	SMPL
L4595-01 - 1	SU-03-111120	3465	0.6824	-7471B	PPB		12 Nov 2020 14:18:33	U	SMPL
CCV21 - 1	CCV21	26841	5.3520	-7471B	PPB		12 Nov 2020 14:20:48	U	SMPL
CCB21 - 1	CCB21	-31	-0.0159	-7471B	PPB		12 Nov 2020 14:23:03	U	SMPL
L4699-01 - 1	STOCKPILE	14673	2.9213	-7471B	PPB		12 Nov 2020 14:25:18	U	SMPL
L4702-01 - 1	M-5(0-10)	1603	0.3105	-7471B	PPB		12 Nov 2020 14:27:33	U	SMPL
L4702-02 - 1	M-5(10-20)	400	0.0702	-7471B	PPB		12 Nov 2020 14:29:48	U	SMPL
L4702-03 - 1	M-6(0-10)	92730	18.5139	-7471B	PPB		12 Nov 2020 14:32:05	U	SMPL
L4702-04 - 1	M-99(0-10)	39248	7.8304	-7471B	PPB		12 Nov 2020 14:34:20	U	SMPL
L4704-01 - 1	KL-SOIL	13681	2.7232	-7471B	PPB		12 Nov 2020 14:36:39	U	SMPL
L4706-01 - 1	COMP-30706-30707-40854	44	-0.0010	-7471B	PPB		12 Nov 2020 14:38:56	U	SMPL
L4706-02 - 1	16874	5142	1.0174	-7471B	PPB		12 Nov 2020 14:41:14	U	SMPL
L4714-01 - 1	EROC-SP-1	10417	2.0711	-7471B	PPB		12 Nov 2020 14:43:30	U	SMPL
L4714-02 - 1	EROC-SP-2	4278	0.8448	-7471B	PPB		12 Nov 2020 14:45:46	U	SMPL
CCV22 - 1	CCV22	26936	5.3710	-7471B	PPB		12 Nov 2020 14:48:02	U	SMPL
CCB22 - 1	CCB22	-26	-0.0149	-7471B	PPB		12 Nov 2020 14:50:17	U	SMPL
L4715-01 - 1	M-6(10-20)	18172	3.6203	-7471B	PPB		12 Nov 2020 14:52:33	U	SMPL
L4716-01 - 1	STOCKPILE-1	11015	2.1906	-7471B	PPB		12 Nov 2020 14:54:48	U	SMPL
L4717-01 - 1	R-LA-35-3-WC	3289	0.6473	-7471B	PPB		12 Nov 2020 14:57:06	U	SMPL
L4718-01 - 1	R-LA-38-1-WC	2514	0.4924	-7471B	PPB		12 Nov 2020 14:59:22	U	SMPL
L4719-03 - 1	TP-3-S	2365	0.4627	-7471B	PPB		12 Nov 2020 15:01:39	U	SMPL
L4719-07 - 1	TP-3-D	770	0.1441	-7471B	PPB		12 Nov 2020 15:03:55	U	SMPL
L4719-11 - 1	TP-3A-S	2514	0.4924	-7471B	PPB		12 Nov 2020 15:06:11	U	SMPL
L4587-01LX5 - 1		559	0.1019	-7471B	PPB		12 Nov 2020 15:08:28	U	SMPL
L4587-01A - 1		26402	5.2643	-7471B	PPB		12 Nov 2020 15:10:45	U	SMPL
L4702-03DLX5 - 1		18830	3.7517	-7471B	PPB		12 Nov 2020 15:13:00	U	SMPL
CCV23 - 1	CCV23	27316	5.4469	-7471B	PPB		12 Nov 2020 15:15:16	U	SMPL
CCB23 - 1	CCB23	-28	-0.0153	-7471B	PPB		12 Nov 2020 15:17:31	U	SMPL