


LB111969

7471B

INSTRUMENT ID: CV1

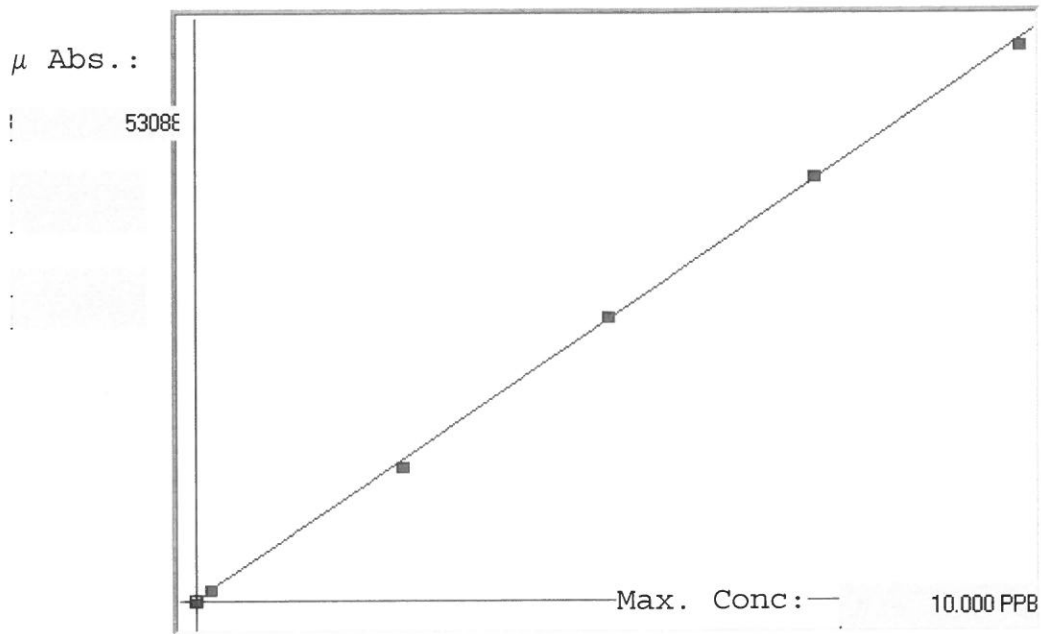

Linear

A= 0.0000e+000

B= 1.8665e-004

C= -7.7976e-003

Rho= 0.9997736

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.000	0.000	43	0.000	43				
0.2	0.200	0.205	0.005	1138	0.0 %	1138				
2.5	2.500	2.404	-0.096	12922	0.0 %	12922				
5.0	5.000	5.094	0.094	27331	0.0 %	27331				
7.5	7.500	7.596	0.096	40739	0.0 %	40739				
10.0	10.000	9.901	-0.099	53088	0.0 %	53088				

LB111969 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 13 Nov 2020 15:13:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	43	-	0.0000	7471B	PPB	13 Nov 2020 15:17:56	S	Std
0.2 - 1	50.2	1138	-	0.2000	7471B	PPB	13 Nov 2020 15:20:13	S	Std
2.5 - 1	52.5	12922	-	2.5000	7471B	PPB	13 Nov 2020 15:22:30	S	Std
5.0 - 1	55	27331	-	5.0000	7471B	PPB	13 Nov 2020 15:24:47	S	Std
7.5 - 1	57.5	40739	-	7.5000	7471B	PPB	13 Nov 2020 15:27:03	S	Std
10.0 - 1	510	53088	-	10.0000	7471B	PPB	13 Nov 2020 15:31:49	S	Std
ICV04 - 1	ICV04	20983	3.9087	-	7471B	PPB	13 Nov 2020 15:34:33	U	SMPL
ICB04 - 1	ICB04	-53	-0.0177	-	7471B	PPB	13 Nov 2020 15:36:48	U	SMPL
CCV31 - 1	CCV31	27697	5.1619	-	7471B	PPB	13 Nov 2020 15:39:03	U	SMPL
CCB31 - 1	CCB31	-57	-0.0184	-	7471B	PPB	13 Nov 2020 15:41:18	U	SMPL
CRA - 1	CRA	1124	0.2020	-	7471B	PPB	13 Nov 2020 15:43:34	U	SMPL
HighStd - 1	HighStd	53088	9.9012	-	7471B	PPB	13 Nov 2020 15:45:49	U	SMPL
ChkStd - 1	ChkStd	37914	7.0689	-	7471B	PPB	13 Nov 2020 15:48:04	U	SMPL
PB132981BL - 1	PBS	-87	-0.0240	-	7471B	PPB	13 Nov 2020 15:50:21	U	SMPL
PB132981BS - 1	LCSS	19038	3.5457	-	7471B	PPB	13 Nov 2020 15:52:38	U	SMPL
L4586-01 - 1	R-LA-33-4-WC	1902	0.3472	-	7471B	PPB	13 Nov 2020 15:59:49	U	SMPL
L4586-01DUP - 1	R-LA-33-4-WCDUP	1846	0.3368	-	7471B	PPB	13 Nov 2020 16:02:05	U	SMPL
L4586-01MS - 1	R-LA-33-4-WCMS	20441	3.8076	-	7471B	PPB	13 Nov 2020 16:04:22	U	SMPL
L4586-01MSD - 1	R-LA-33-4-WCMSD	20771	3.8692	-	7471B	PPB	13 Nov 2020 16:06:39	U	SMPL
L4723-02 - 1	RBR-59	1173	0.2111	-	7471B	PPB	13 Nov 2020 16:08:54	U	SMPL
CCV32 - 1	CCV32	27232	5.0751	-	7471B	PPB	13 Nov 2020 16:11:10	U	SMPL
CCB32 - 1	CCB32	-50	-0.0171	-	7471B	PPB	13 Nov 2020 16:13:25	U	SMPL
L4725-02 - 1	RBR-31	1537	0.2791	-	7471B	PPB	13 Nov 2020 16:15:40	U	SMPL
L4725-04 - 1	RBR-34	1077	0.1932	-	7471B	PPB	13 Nov 2020 16:17:55	U	SMPL
L4735-01 - 1	R-LA-33-3-WC	3330	0.6138	-	7471B	PPB	13 Nov 2020 16:20:10	U	SMPL
L4586-01LX5 - 1		365	0.0603	-	7471B	PPB	13 Nov 2020 16:22:26	U	SMPL
L4586-01A - 1		22675	4.2245	-	7471B	PPB	13 Nov 2020 16:24:41	U	SMPL
CCV33 - 1	CCV33	27366	5.1001	-	7471B	PPB	13 Nov 2020 16:26:58	U	SMPL
CCB33 - 1	CCB33	-41	-0.0155	-	7471B	PPB	13 Nov 2020 16:29:14	U	SMPL