


LB111982

7471B

INSTRUMENT ID: CY1

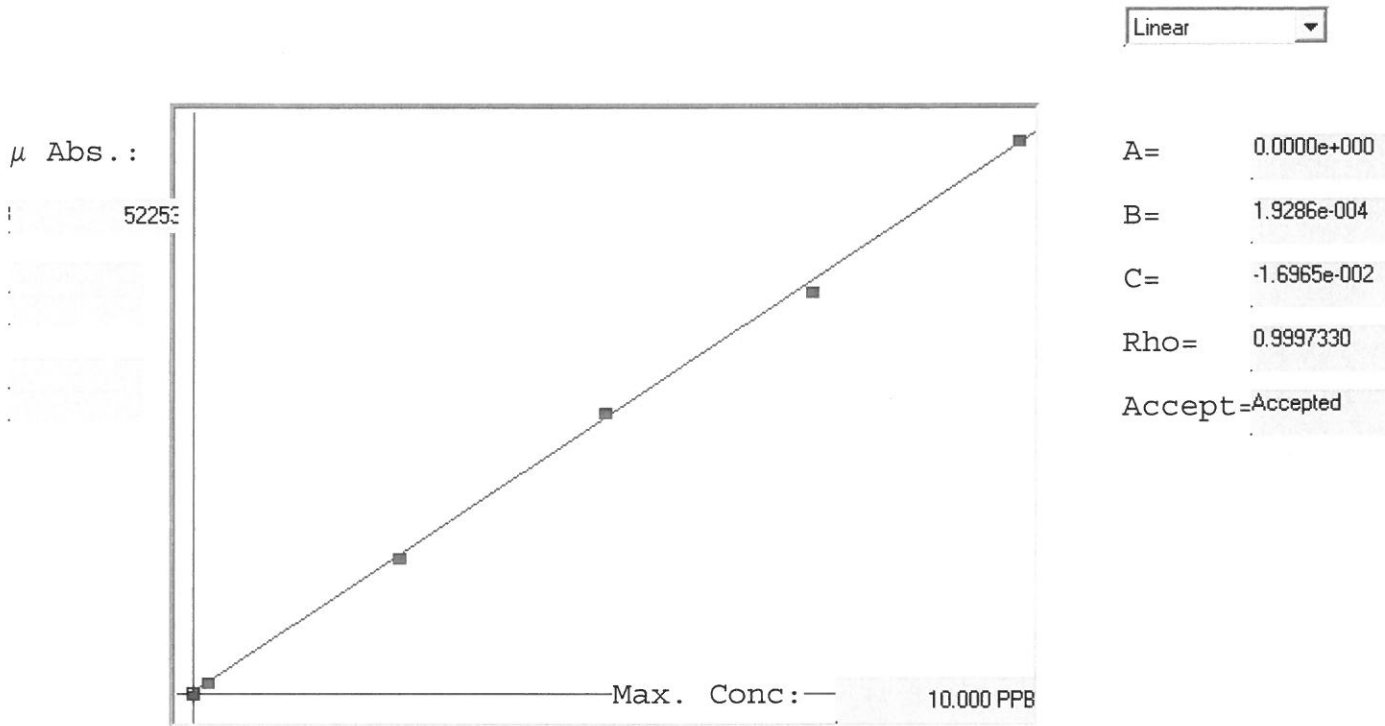

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.001	0.001	95	0.000	95				
0.2	0.200	0.195	-0.005	1097	0.0 %	1097				
2.5	2.500	2.486	-0.014	12977	0.0 %	12977				
5.0	5.000	5.118	0.118	26626	0.0 %	26626				
7.5	7.500	7.340	-0.160	38144	0.0 %	38144				
10.0	10.000	10.061	0.061	52253	0.0 %	52253				

LB111982 INSTRUMENT ID: CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Nov 2020 12:12:26

Sample ID	Extended ID	μ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	95	-	0.00007471B	PPB	16 Nov 2020 12:13:42	S	Std
0.2 - 1	50.2	1097	-	0.20007471B	PPB	16 Nov 2020 12:15:58	S	Std
2.5 - 1	52.5	12977	-	2.50007471B	PPB	16 Nov 2020 12:18:15	S	Std
5.0 - 1	55	26626	-	5.00007471B	PPB	16 Nov 2020 12:20:32	S	Std
7.5 - 1	57.5	38144	-	7.50007471B	PPB	16 Nov 2020 12:22:49	S	Std
10.0 - 1	59	52253	-	10.00007471B	PPB	16 Nov 2020 12:25:05	S	Std
ICV05 - 1	ICV05	19969	3.8343	-7471B	PPB	16 Nov 2020 12:31:47	U	SMPL
ICB05 - 1	ICB05	-1	-0.0172	-7471B	PPB	16 Nov 2020 12:34:02	U	SMPL
CCV37 - 1	CCV37	26289	5.0532	-7471B	PPB	16 Nov 2020 12:36:17	U	SMPL
CCB37 - 1	CCB37	-40	-0.0247	-7471B	PPB	16 Nov 2020 12:38:32	U	SMPL
CRA - 1	CRA	1080	0.1913	-7471B	PPB	16 Nov 2020 12:40:47	U	SMPL
HighStd - 1	HighStd	51904	9.9933	-7471B	PPB	16 Nov 2020 12:43:02	U	SMPL
ChkStd - 1	ChkStd	36598	7.0414	-7471B	PPB	16 Nov 2020 12:45:17	U	SMPL
PB133025BL - 1	PBS	-117	-0.0395	-7471B	PPB	16 Nov 2020 12:47:34	U	SMPL
PB133025BS - 1	LCSS	17653	3.3876	-7471B	PPB	16 Nov 2020 12:49:51	U	SMPL
L4734-01 - 1	BARNUM-STREET-TEST-PIT-1	31247	6.0094	-7471B	PPB	16 Nov 2020 12:52:08	U	SMPL
L4734-02 - 1	BARNUM-STREET-TEST-PIT-2	43319	8.3376	-7471B	PPB	16 Nov 2020 12:54:24	U	SMPL
L4745-01 - 1	CV-OS	105	0.0033	-7471B	PPB	16 Nov 2020 12:56:42	U	SMPL
L4746-01 - 1	OK-02-111320	2365	0.4392	-7471B	PPB	16 Nov 2020 12:59:00	U	SMPL
L4746-01DUP - 1	OK-02-111320DUP	2267	0.4203	-7471B	PPB	16 Nov 2020 13:04:01	U	SMPL
CCV38 - 1	CCV38	26186	5.0333	-7471B	PPB	16 Nov 2020 13:06:16	U	SMPL
CCB38 - 1	CCB38	-1	-0.0172	-7471B	PPB	16 Nov 2020 13:08:30	U	SMPL
L4746-01MS - 1	OK-02-111320MS	19658	3.7743	-7471B	PPB	16 Nov 2020 13:10:45	U	SMPL
L4746-01MSD - 1	OK-02-111320MSD	21563	4.1417	-7471B	PPB	16 Nov 2020 13:13:00	U	SMPL
L4746-01LX5 - 1		491	0.0777	-7471B	PPB	16 Nov 2020 13:15:16	U	SMPL
L4746-01A - 1		22810	4.3822	-7471B	PPB	16 Nov 2020 13:17:32	U	SMPL
CCV39 - 1	CCV39	26343	5.0636	-7471B	PPB	16 Nov 2020 13:19:48	U	SMPL
CCB39 - 1	CCB39	-13	-0.0195	-7471B	PPB	16 Nov 2020 13:22:04	U	SMPL