


LB112006

7471B

INSTRUMENT ID: CV1

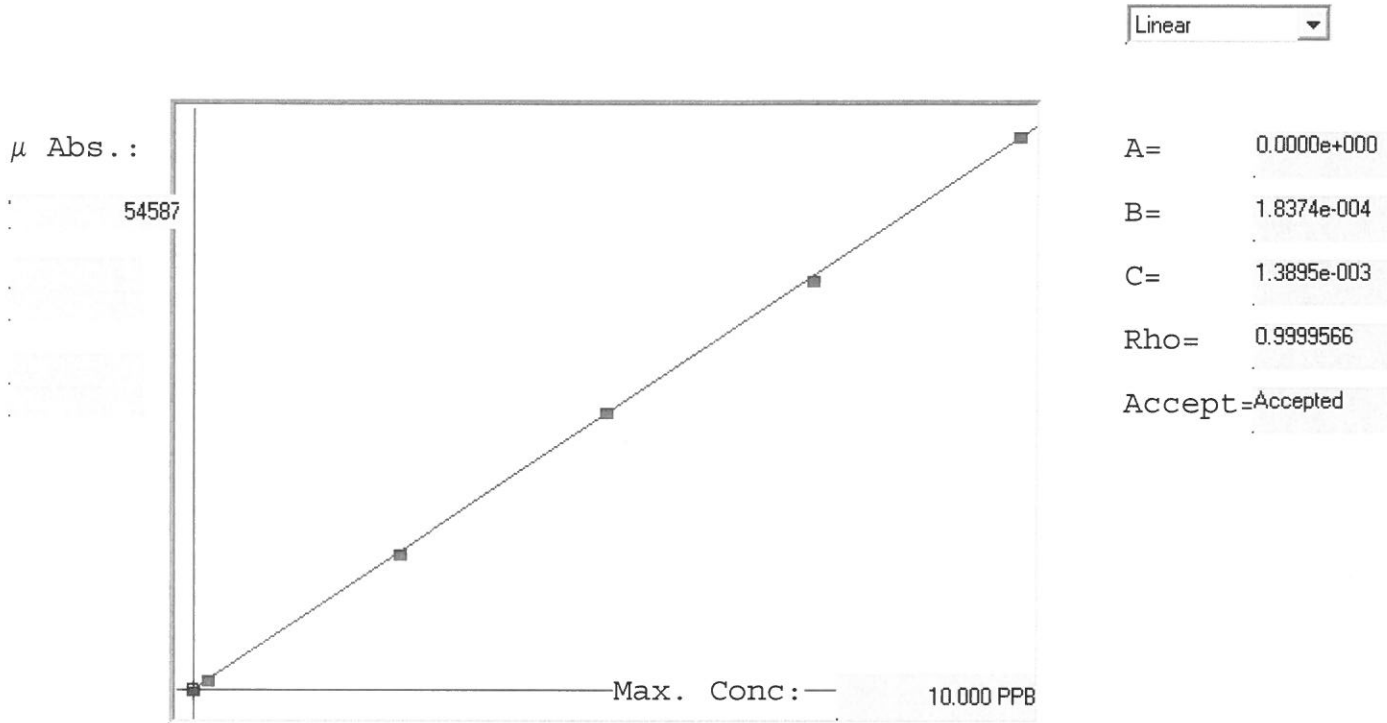

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.009	0.009	44	0.000	44				
0.2	0.200	0.195	-0.005	1051	0.0 %	1051				
2.5	2.500	2.491	-0.009	13550	0.0 %	13550				
5.0	5.000	5.040	0.040	27420	0.0 %	27420				
7.5	7.500	7.434	-0.066	40452	0.0 %	40452				
10.0	10.000	10.031	0.031	54587	0.0 %	54587				

LB112006 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 17 Nov 2020 12:41:47

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	44	-	0.00007471B	PPB	17 Nov 2020 13:14:54	S	Std
0.2 - 1	50.2	1051	-	0.20007471B	PPB	17 Nov 2020 13:17:12	S	Std
2.5 - 1	52.5	13550	-	2.50007471B	PPB	17 Nov 2020 13:19:29	S	Std
5.0 - 1	55	27420	-	5.00007471B	PPB	17 Nov 2020 13:21:46	S	Std
7.5 - 1	57.5	40452	-	7.50007471B	PPB	17 Nov 2020 13:24:02	S	Std
10.0 - 1	510	54587	-	10.00007471B	PPB	17 Nov 2020 13:26:18	S	Std
ICV07 - 1	ICV07	20817	3.8263	-7471B	PPB	17 Nov 2020 13:29:00	U	SMPL
ICB07 - 1	ICB07	-59	-0.0095	-7471B	PPB	17 Nov 2020 13:31:15	U	SMPL
CCV44 - 1	CCV44	27499	5.0541	-7471B	PPB	17 Nov 2020 13:33:30	U	SMPL
CCB44 - 1	CCB44	-75	-0.0124	-7471B	PPB	17 Nov 2020 13:35:45	U	SMPL
CRA - 1	CRA	1044	0.1932	-7471B	PPB	17 Nov 2020 13:38:00	U	SMPL
HighStd - 1	HighStd	53803	9.8872	-7471B	PPB	17 Nov 2020 13:40:15	U	SMPL
ChkStd - 1	ChkStd	34732	6.3831	-7471B	PPB	17 Nov 2020 13:42:30	U	SMPL
PB133048BL - 1	PBS	-113	-0.0194	-7471B	PPB	17 Nov 2020 13:44:48	U	SMPL
PB133048BS - 1	LCSS	18809	3.4574	-7471B	PPB	17 Nov 2020 13:47:05	U	SMPL
L4768-01 - 1	TR-05-111620	2956	0.5445	-7471B	PPB	17 Nov 2020 13:49:21	U	SMPL
L4769-10 - 1	ETGI-359	256	0.0484	-7471B	PPB	17 Nov 2020 13:51:38	U	SMPL
L4770-01 - 1	FJ-BH-01-0-1	2813	0.5183	-7471B	PPB	17 Nov 2020 13:53:55	U	SMPL
L4770-03 - 1	FJ-BH-01-2-3	1684	0.3108	-7471B	PPB	17 Nov 2020 13:56:13	U	SMPL
L4770-05 - 1	FJ-BH-01-4-5	595	0.1107	-7471B	PPB	17 Nov 2020 13:58:28	U	SMPL
CCV45 - 1	CCV45	27018	4.9657	-7471B	PPB	17 Nov 2020 14:00:43	U	SMPL
CCB45 - 1	CCB45	-75	-0.0124	-7471B	PPB	17 Nov 2020 14:02:59	U	SMPL
L4770-07 - 1	FJ-BH-02-0-1	6015	1.1066	-7471B	PPB	17 Nov 2020 14:05:14	U	SMPL
L4770-09 - 1	FJ-BH-02-2-3	5745	1.0570	-7471B	PPB	17 Nov 2020 14:07:30	U	SMPL
L4770-11 - 1	FJ-BH-02-4-5	792	0.1469	-7471B	PPB	17 Nov 2020 14:09:45	U	SMPL
L4770-13 - 1	FJ-BH-03-0-1	3423	0.6303	-7471B	PPB	17 Nov 2020 14:12:01	U	SMPL
L4770-15 - 1	FJ-BH-03-2-3	10433	1.9184	-7471B	PPB	17 Nov 2020 14:14:16	U	SMPL
L4770-17 - 1	FJ-BH-03-4-5	186	0.0356	-7471B	PPB	17 Nov 2020 14:16:33	U	SMPL
L4770-19 - 1	FJ-BH-04-0-1	2728	0.5026	-7471B	PPB	17 Nov 2020 14:18:49	U	SMPL
L4770-21 - 1	FJ-BH-04-2-3	2130	0.3928	-7471B	PPB	17 Nov 2020 14:21:06	U	SMPL
L4770-23 - 1	FJ-BH-04-4-5	864	0.1601	-7471B	PPB	17 Nov 2020 14:23:23	U	SMPL
L4771-01 - 1	CD-BH-01-0-1	7127	1.3109	-7471B	PPB	17 Nov 2020 14:25:39	U	SMPL
CCV46 - 1	CCV46	27530	5.0598	-7471B	PPB	17 Nov 2020 14:27:55	U	SMPL
CCB46 - 1	CCB46	-32	-0.0045	-7471B	PPB	17 Nov 2020 14:30:11	U	SMPL
L4771-03 - 1	CD-BH-01-2-3	1167	0.2158	-7471B	PPB	17 Nov 2020 14:32:26	U	SMPL
L4771-05 - 1	CD-BH-01-4-5	659	0.1225	-7471B	PPB	17 Nov 2020 14:34:42	U	SMPL
L4771-07 - 1	CD-BH-02-0-1	5062	0.9315	-7471B	PPB	17 Nov 2020 14:36:57	U	SMPL
L4771-09 - 1	CD-BH-02-2-3	982	0.1818	-7471B	PPB	17 Nov 2020 14:39:13	U	SMPL
L4771-09DUP - 1	CD-BH-02-2-3DUP	939	0.1739	-7471B	PPB	17 Nov 2020 14:41:28	U	SMPL
L4771-09MS - 1	CD-BH-02-2-3MS	20938	3.8486	-7471B	PPB	17 Nov 2020 14:43:45	U	SMPL
L4771-09MSD - 1	CD-BH-02-2-3MSD	20803	3.8238	-7471B	PPB	17 Nov 2020 14:46:01	U	SMPL
L4771-11 - 1	CD-BH-02-4-5	718	0.1333	-7471B	PPB	17 Nov 2020 14:48:18	U	SMPL
L4771-09LX5 - 1		193	0.0369	-7471B	PPB	17 Nov 2020 14:50:34	U	SMPL
L4771-09A - 1		22025	4.0483	-7471B	PPB	17 Nov 2020 14:52:50	U	SMPL
CCV47 - 1	CCV47	27775	5.1048	-7471B	PPB	17 Nov 2020 14:55:06	U	SMPL
CCB47 - 1	CCB47	-57	-0.0091	-7471B	PPB	17 Nov 2020 14:57:22	U	SMPL