


LB112084

ISM02.4

INSTRUMENT ID: CV1

 μ Abs.:

45804

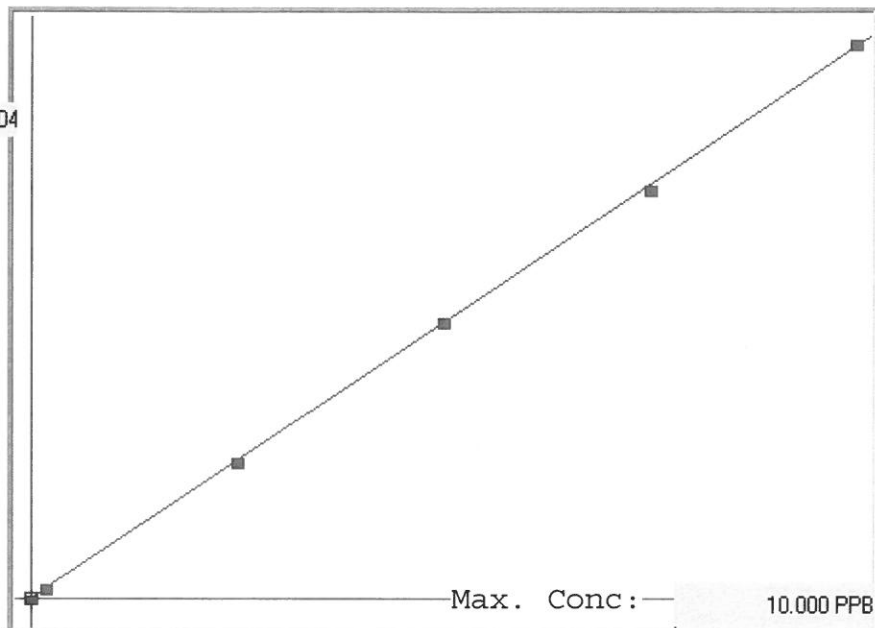

Linear

A= 0.0000e+000

B= 2.1925e-004

C= -2.6579e-003

Rho= 0.9999551

Accept=Accepted

done
 $y = 10x + \text{intercept}$

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	U/D
0.00	0.000	0.013	0.013	71	0.000	71					1
0.05	0.050					244					-3
0.20	0.200	0.195	-0.005	900	0.0 %	900					0
2.50	2.500	2.497	-0.003	11402	0.0 %	11402					0
5.00	5.000	5.025	0.025	22932	0.0 %	22932					-1
7.50	7.500	7.430	-0.070	33900	0.0 %	33900					-1
10.0	10.000	10.040	0.040	45804	0.0 %	45804					0

LB112084
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	71	-		0 ISM02.4	PPB	11/20/2020 17:02	Std
	0.2 S0.2	900	-		0.2 ISM02.4	PPB	11/20/2020 17:04	Std
	2.5 S2.5	11402	-		2.5 ISM02.4	PPB	11/20/2020 17:06	Std
	5 S5.0	22932	-		5 ISM02.4	PPB	11/20/2020 17:08	Std
	7.5 S7.5	33900	-		7.5 ISM02.4	PPB	11/20/2020 17:11	Std
	10 S10.0	45804	-		10 ISM02.4	PPB	11/20/2020 17:13	Std
ICV	ICV	17304	3.7913	-	ISM02.4	PPB	11/20/2020 17:16	SMPL
ICB	ICB	-46	-0.0127	-	ISM02.4	PPB	11/20/2020 17:18	SMPL
CCV071	CCV071	22914	5.0213	-	ISM02.4	PPB	11/20/2020 17:20	SMPL
CCB071	CCB071	-54	-0.0145	-	ISM02.4	PPB	11/20/2020 17:22	SMPL
PB133158BL	PBS158	22	0.0022	-	ISM02.4	PPB	11/20/2020 17:25	SMPL
L4852-01	MCOAD0	1897	0.4133	-	ISM02.4	PPB	11/20/2020 17:27	SMPL
L4852-02	MCOAD1	4484	0.9805	-	ISM02.4	PPB	11/20/2020 17:29	SMPL
L4852-03	MCOAD2	1997	0.4352	-	ISM02.4	PPB	11/20/2020 17:36	SMPL
L4852-04	MCOAD2D	2028	0.442	-	ISM02.4	PPB	11/20/2020 17:38	SMPL
L4852-05	MCOAD2S	12569	2.7531	-	ISM02.4	PPB	11/20/2020 17:41	SMPL
L4852-06	MCOAD4	1706	0.3714	-	ISM02.4	PPB	11/20/2020 17:43	SMPL
CCV072	CCV072	22213	4.8676	-	ISM02.4	PPB	11/20/2020 17:45	SMPL
CCB072	CCB072	-27	-0.0086	-	ISM02.4	PPB	11/20/2020 17:48	SMPL