

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : MA

Instrument ID : Konelab

11/23/2020 11:22

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.845	0.0	0.085	
ICB1	0.586	0.0	0.001	
CCV1	245.070	0.0	0.216	
CCB1	0.404	0.0	0.000	
PB133142BL	0.343	0.0	0.000	
L4786-02	0.277	0.0	0.000	
L4786-02DUP	0.214	0.0	0.000	
L4807-01	0.260	0.0	0.000	
L4826-01	0.224	0.0	0.000	
L4845-04	0.670	0.0	0.001	
L4858-03	0.293	0.0	0.000	
L4858-04	0.200	0.0	0.000	
CCV2	249.907	0.0	0.220	
CCB2	0.242	0.0	0.000	
L4826-02	0.318	0.0	0.000	
L4826-02DUP	0.295	0.0	0.000	
PB133143BL	0.216	0.0	0.000	
CCV3	260.489	0.0	0.230	
CCB3	0.382	0.0	0.000	

N	19
Mean	45.065
SD	94.5660
CV%	209.84

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

11/23/2020 8:54

Test *Reactive* Total CN *AL*

11/23/20


Accepted 11/23/2020 8:54

Factor 1134

Bias 0

Coeff. of det. 0.999953

Errors

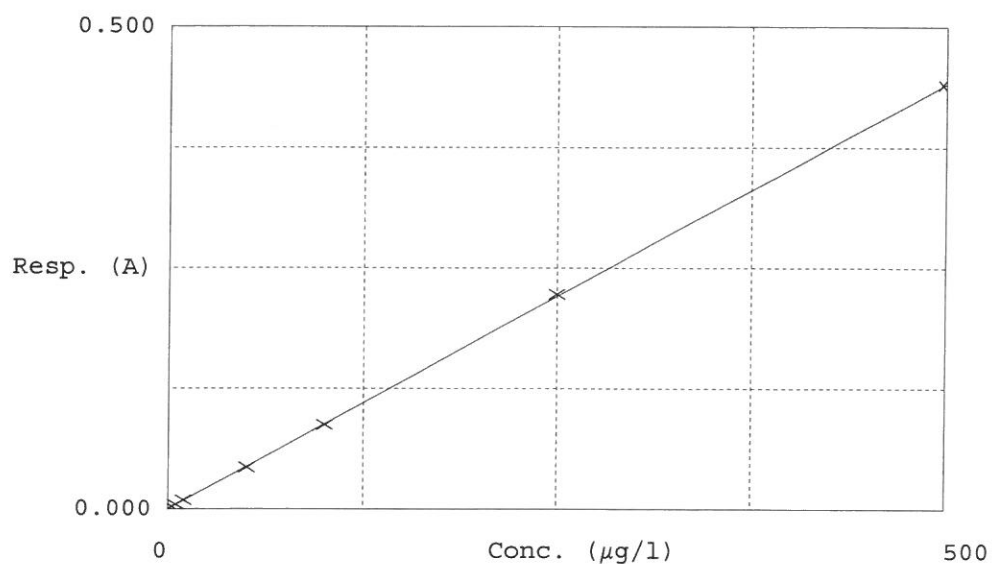

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.1044	0.0000	
2	5.0PPBCN	0.004	4.8455	5.0000	
3	10PPBCN	0.009	10.5028	10.0000	
4	50PPBCN	0.043	48.9868	50.0000	
5	100PPBCN	0.087	99.0029	100.0000	
6	250PPBCN	0.223	252.5307	250.0000	
7	500PPBCN	0.440	499.0269	500.0000	

11/23/20

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 23 08:54:18 2020

Mon Nov 23 11:22:10 2020

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.1044	µg/l	11/23/2020 8:54:18	
5.OPPBCN	A	Reactive CN	P	4.8455	µg/l	11/23/2020 8:54:19	
10PPBCN	A	Reactive CN	P	10.5028	µg/l	11/23/2020 8:54:20	
50PPBCN	A	Reactive CN	P	48.9868	µg/l	11/23/2020 8:54:21	
100PPBCN	A	Reactive CN	P	99.0029	µg/l	11/23/2020 8:54:22	
250PPBCN	A	Reactive CN	P	252.5307	µg/l	11/23/2020 8:54:23	
500PPBCN	A	Reactive CN	P	499.0269	µg/l	11/23/2020 8:54:24	
ICV1	S	Reactive CN	P	95.8449	µg/l	11/23/2020 10:59:44	
ICB1	S	Reactive CN	P	0.5856	µg/l	11/23/2020 10:59:45	
CCV1	S	Reactive CN	P	245.07	µg/l	11/23/2020 10:59:46	
CCB1	S	Reactive CN	P	0.4044	µg/l	11/23/2020 10:59:47	
PB133142BL	S	Reactive CN	P	0.3432	µg/l	11/23/2020 10:59:48	
L4786-02	S	Reactive CN	P	0.2773	µg/l	11/23/2020 10:59:49	
L4786-02DUP	S	Reactive CN	P	0.2136	µg/l	11/23/2020 10:59:50	
L4807-01	S	Reactive CN	P	0.2595	µg/l	11/23/2020 10:59:51	
L4826-01	S	Reactive CN	P	0.2243	µg/l	11/23/2020 10:59:52	
L4845-04	S	Reactive CN	P	0.6701	µg/l	11/23/2020 10:59:53	
L4858-03	S	Reactive CN	P	0.2928	µg/l	11/23/2020 10:59:54	
L4858-04	S	Reactive CN	P	0.2003	µg/l	11/23/2020 11:05:55	
CCV2	S	Reactive CN	P	249.9069	µg/l	11/23/2020 11:05:56	
CCB2	S	Reactive CN	P	0.2417	µg/l	11/23/2020 11:05:57	
L4826-02	S	Reactive CN	P	0.3177	µg/l	11/23/2020 11:05:59	
L4826-02DUP	S	Reactive CN	P	0.2952	µg/l	11/23/2020 11:06:00	
PB133143BL	S	Reactive CN	P	0.2165	µg/l	11/23/2020 11:22:08	
CCV3	S	Reactive CN	P	260.4886	µg/l	11/23/2020 11:22:09	
CCB3	S	Reactive CN	P	0.3825	µg/l	11/23/2020 11:22:10	