

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : M

Instrument ID : Konelab

11/25/2020 11:47

Test: *Leach* Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.496	0.0	0.083	
ICB1	1.595	0.0	0.001	
CCV1	252.277	0.0	0.215	
CCB1	1.980	0.0	0.002	
PB133262BL	2.229	0.0	0.002	
L4597-04	1.834	0.0	0.001	
L4597-04DUP	1.488	0.0	0.001	
L4882-04	1.741	0.0	0.001	
L4882-06	1.768	0.0	0.001	
L4884-01	0.856	0.0	0.001	
L4891-04	1.793	0.0	0.001	
L4891-06	1.848	0.0	0.001	
CCV2	257.088	0.0	0.219	
CCB2	1.510	0.0	0.001	

N	14
Mean	44.679
SD	92.5408
CV%	207.12



Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 25 09:42:44 2020

Wed Nov 25 11:46:34 2020

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.9241	µg/l	11/25/2020 9:42:44	
5.0PPBCN	A	Reactive CN	P	5.0909	µg/l	11/25/2020 9:42:45	
10PPBCN	A	Reactive CN	P	10.8814	µg/l	11/25/2020 9:42:46	
50PPBCN	A	Reactive CN	P	48.1732	µg/l	11/25/2020 9:42:47	
100PPBCN	A	Reactive CN	P	98.8638	µg/l	11/25/2020 9:42:48	
250PPBCN	A	Reactive CN	P	251.3506	µg/l	11/25/2020 9:42:49	
500PPBCN	A	Reactive CN	P	499.7161	µg/l	11/25/2020 9:42:50	
ICV1	S	Reactive CN	P	97.4963	µg/l	11/25/2020 11:25:12	
ICB1	S	Reactive CN	P	1.5948	µg/l	11/25/2020 11:25:13	
CCV1	S	Reactive CN	P	252.2771	µg/l	11/25/2020 11:25:16	
CCB1	S	Reactive CN	P	1.9801	µg/l	11/25/2020 11:25:18	
PB133262BL	S	Reactive CN	P	2.2288	µg/l	11/25/2020 11:25:19	
L4597-04	S	Reactive CN	P	1.8342	µg/l	11/25/2020 11:25:20	
L4597-04DUP	S	Reactive CN	P	1.4883	µg/l	11/25/2020 11:25:21	
L4882-04	S	Reactive CN	P	1.741	µg/l	11/25/2020 11:30:54	
L4882-06	S	Reactive CN	P	1.7682	µg/l	11/25/2020 11:30:55	
L4884-01	S	Reactive CN	P	0.8561	µg/l	11/25/2020 11:30:56	
L4891-04	S	Reactive CN	P	1.7926	µg/l	11/25/2020 11:30:57	
L4891-06	S	Reactive CN	P	1.8484	µg/l	11/25/2020 11:30:58	
CCV2	S	Reactive CN	P	257.0877	µg/l	11/25/2020 11:46:32	
CCB2	S	Reactive CN	P	1.5103	µg/l	11/25/2020 11:46:33	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Al

Instrument ID : Konelab

11/25/2020 9:43


Test ^{Reactive}
Total CN

Accepted 11/25/2020 9:43

Factor 1174
Bias 0

Coeff. of det. 0.999960

Errors

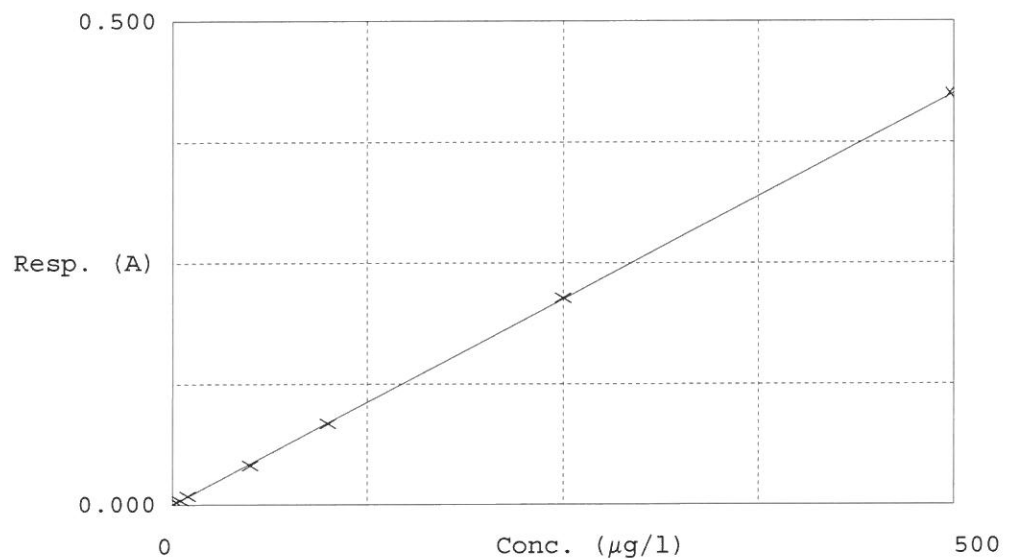

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.9241	0.0000	
2	5.0PPBCN	0.004	5.0909	5.0000	
3	10PPBCN	0.009	10.8814	10.0000	
4	50PPBCN	0.041	48.1732	50.0000	
5	100PPBCN	0.084	98.8638	100.0000	
6	250PPBCN	0.214	251.3506	250.0000	
7	500PPBCN	0.425	499.7161	500.0000	