


LB112189

7470A

INSTRUMENT ID: CV1

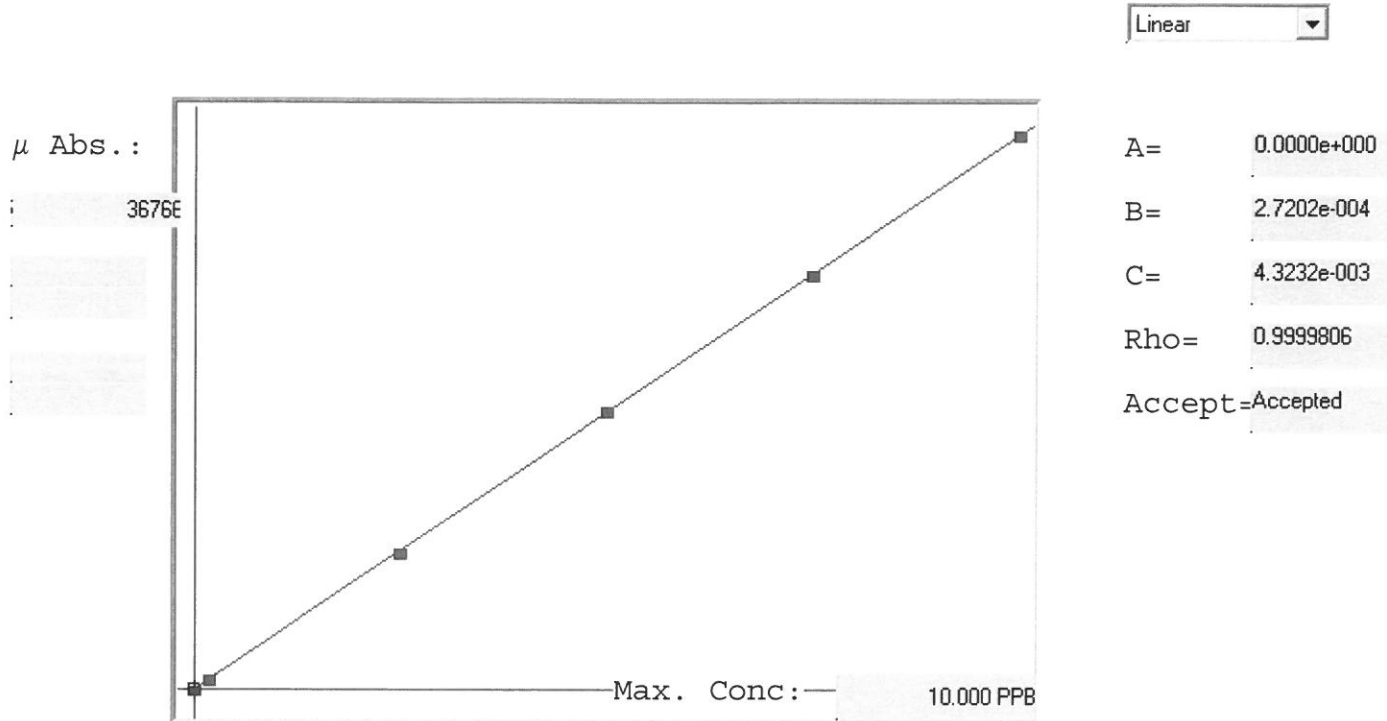

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.006	0.006	7	0.000	7				
0.2	0.200	0.209	0.009	754	0.0 %	754				
2.5	2.500	2.463	-0.037	9037	0.0 %	9037				
5.0	5.000	5.035	0.035	18495	0.0 %	18495				
7.5	7.500	7.481	-0.019	27485	0.0 %	27485				
10.0	10.000	10.006	0.006	36766	0.0 %	36766				

LB112189 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Dec 2020 12:14:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	7	-	0.0000	7470A	PPB	02 Dec 2020 12:25:06	S	Std
0.2 - 1	50.2	754	-	0.2000	7470A	PPB	02 Dec 2020 12:27:24	S	Std
2.5 - 1	52.5	9037	-	2.5000	7470A	PPB	02 Dec 2020 12:29:41	S	Std
5.0 - 1	55	18495	-	5.0000	7470A	PPB	02 Dec 2020 12:31:58	S	Std
7.5 - 1	57.5	27485	-	7.5000	7470A	PPB	02 Dec 2020 12:34:14	S	Std
10.0 - 1	51.8	36766	-	10.0000	7470A	PPB	02 Dec 2020 12:36:30	S	Std
ICV24 - 1	ICV24	14403	3.9223	-	7470A	PPB	02 Dec 2020 12:39:21	U	SMPL
ICB24 - 1	ICB24	-69	-0.0144	-	7470A	PPB	02 Dec 2020 12:41:36	U	SMPL
CCV16 - 1	CCV16	18775	5.1115	-	7470A	PPB	02 Dec 2020 12:43:51	U	SMPL
CCB16 - 1	CCB16	-67	-0.0139	-	7470A	PPB	02 Dec 2020 12:46:06	U	SMPL
CRA - 1	CRA	746	0.2073	-	7470A	PPB	02 Dec 2020 12:48:21	U	SMPL
HighStd - 1	HighStd	36358	9.8945	-	7470A	PPB	02 Dec 2020 12:50:36	U	SMPL
ChkStd - 1	ChkStd	25460	6.9300	-	7470A	PPB	02 Dec 2020 12:52:51	U	SMPL
PB133352BL - 1	PBW	-105	-0.0242	-	7470A	PPB	02 Dec 2020 12:55:07	U	SMPL
PB133352BS - 1	LCSW	15588	4.2446	-	7470A	PPB	02 Dec 2020 12:57:24	U	SMPL
L4809-15 - 1	MS-CON-A	-48	-0.0087	-	7470A	PPB	02 Dec 2020 12:59:40	U	SMPL
L4809-16 - 1	MS-CON-B	13	0.0079	-	7470A	PPB	02 Dec 2020 13:01:56	U	SMPL
L4809-17 - 1	MS-CON-D	2	0.0049	-	7470A	PPB	02 Dec 2020 13:04:13	U	SMPL
L4809-18 - 1	MS-CON-E	63	0.0215	-	7470A	PPB	02 Dec 2020 13:06:31	U	SMPL
L4809-18DUP - 1	MS-CON-EDUP	115	0.0356	-	7470A	PPB	02 Dec 2020 13:08:46	U	SMPL
CCV17 - 1	CCV17	19059	5.1888	-	7470A	PPB	02 Dec 2020 13:11:01	U	SMPL
CCB17 - 1	CCB17	-65	-0.0134	-	7470A	PPB	02 Dec 2020 13:13:16	U	SMPL
L4809-18MS - 1	MS-CON-EMS	13998	3.8121	-	7470A	PPB	02 Dec 2020 13:15:32	U	SMPL
L4809-18MSD - 1	MS-CON-EMSD	13392	3.6473	-	7470A	PPB	02 Dec 2020 13:17:47	U	SMPL
PB133352TB - 1	PB133336TB	-55	-0.0106	-	7470A	PPB	02 Dec 2020 13:20:03	U	SMPL
L4809-18LX5 - 1		7	0.0062	-	7470A	PPB	02 Dec 2020 13:22:18	U	SMPL
L4809-18A - 1		14863	4.0474	-	7470A	PPB	02 Dec 2020 13:24:34	U	SMPL
CCV18 - 1	CCV18	18676	5.0846	-	7470A	PPB	02 Dec 2020 13:26:50	U	SMPL
CCB18 - 1	CCB18	-71	-0.0150	-	7470A	PPB	02 Dec 2020 13:29:07	U	SMPL