


LB112192

7471B

INSTRUMENT ID: CVL

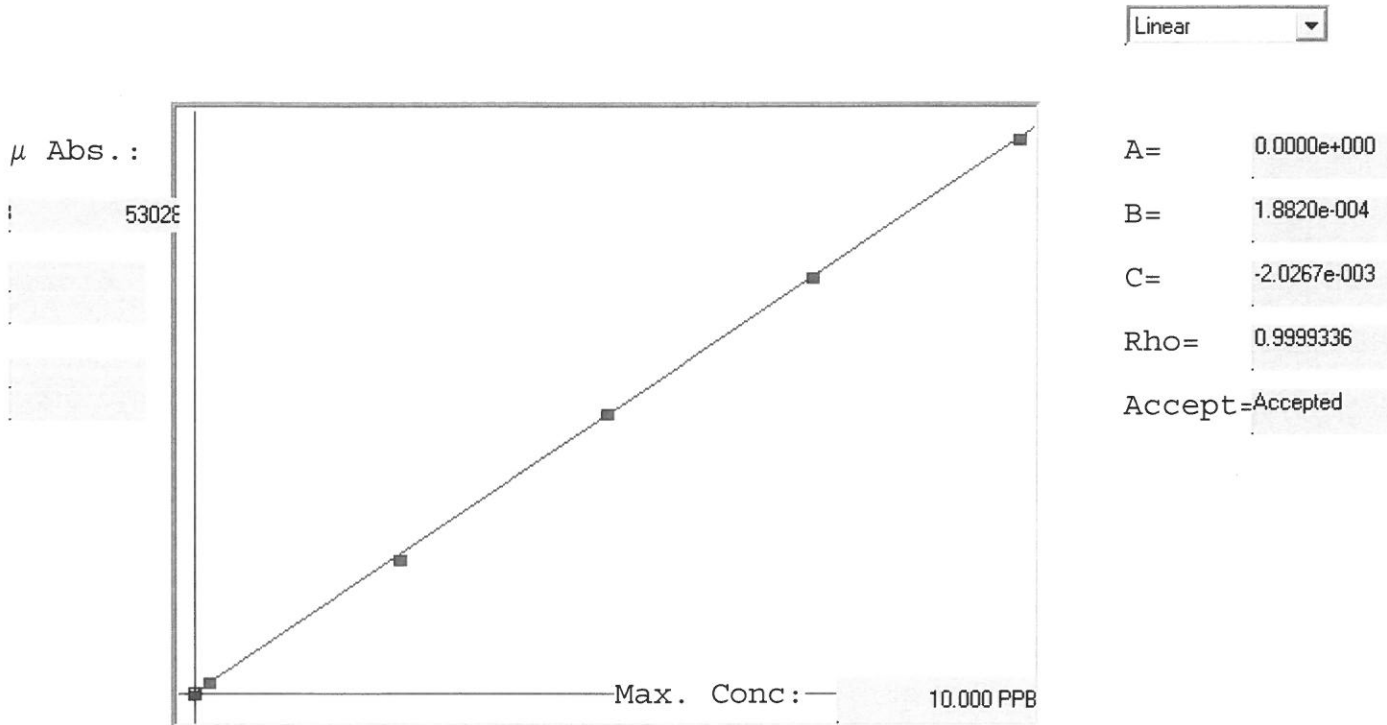

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	2	0.000	2				
0.2	0.200	0.218	0.018	1170	0.0 %	1170				
2.5	2.500	2.431	-0.069	12927	0.0 %	12927				
5.0	5.000	5.072	0.072	26963	0.0 %	26963				
7.5	7.500	7.502	0.002	39873	0.0 %	39873				
10.0	10.000	9.978	-0.022	53028	0.0 %	53028				

LB112192 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Dec 2020 13:43:12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	2	-	0.0000	7471B	PPB	02 Dec 2020 13:43:58	S	Std
0.2 - 1	50.2	1170	-	0.2000	7471B	PPB	02 Dec 2020 13:46:15	S	Std
2.5 - 1	52.5	12927	-	2.5000	7471B	PPB	02 Dec 2020 13:48:32	S	Std
5.0 - 1	55	26963	-	5.0000	7471B	PPB	02 Dec 2020 13:50:49	S	Std
7.5 - 1	57.5	39873	-	7.5000	7471B	PPB	02 Dec 2020 13:53:05	S	Std
10.0 - 1	57.0	53028	-	10.0000	7471B	PPB	02 Dec 2020 13:57:56	S	Std
ICV25 - 1	ICV25	21058	3.9611	-	7471B	PPB	02 Dec 2020 14:00:34	U	SMPL
ICB25 - 1	ICB25	70	0.0111	-	7471B	PPB	02 Dec 2020 14:02:50	U	SMPL
CCV19 - 1	CCV19	27075	5.0936	-	7471B	PPB	02 Dec 2020 14:05:05	U	SMPL
CCB19 - 1	CCB19	80	0.0130	-	7471B	PPB	02 Dec 2020 14:07:20	U	SMPL
CRA - 1	CRA	1130	0.2106	-	7471B	PPB	02 Dec 2020 14:09:35	U	SMPL
HighStd - 1	HighStd	52591	9.8957	-	7471B	PPB	02 Dec 2020 14:11:50	U	SMPL
ChkStd - 1	ChkStd	37839	7.1194	-	7471B	PPB	02 Dec 2020 14:16:41	U	SMPL
PB133351BL - 1	PBS	64	0.0100	-	7471B	PPB	02 Dec 2020 14:18:56	U	SMPL
PB133351BS - 1	LCSS	19002	3.5742	-	7471B	PPB	02 Dec 2020 14:21:13	U	SMPL
L4911-01 - 1	SK-12-1-SPA	9904	1.8619	-	7471B	PPB	02 Dec 2020 14:23:30	U	SMPL
L4911-01DUP - 1	SK-12-1-SPADUP	9259	1.7405	-	7471B	PPB	02 Dec 2020 14:25:46	U	SMPL
L4911-01MS - 1	SK-12-1-SPAMS	34194	6.4334	-	7471B	PPB	02 Dec 2020 14:28:03	U	SMPL
L4911-01MSD - 1	SK-12-1-SPAMSD	30009	5.6457	-	7471B	PPB	02 Dec 2020 14:30:20	U	SMPL
L4911-02 - 1	SK-12-1-SPB	6164	1.1581	-	7471B	PPB	02 Dec 2020 14:32:36	U	SMPL
CCV20 - 1	CCV20	26859	5.0529	-	7471B	PPB	02 Dec 2020 14:34:52	U	SMPL
CCB20 - 1	CCB20	87	0.0143	-	7471B	PPB	02 Dec 2020 14:37:08	U	SMPL
L4911-03 - 1	SK-12-1-SPC	9810	1.8442	-	7471B	PPB	02 Dec 2020 14:39:24	U	SMPL
L4911-04 - 1	SK-12-1-SPD	10387	1.9528	-	7471B	PPB	02 Dec 2020 14:41:39	U	SMPL
L4911-05 - 1	SK-12-1-SPE	2356	0.4414	-	7471B	PPB	02 Dec 2020 14:43:55	U	SMPL
L4913-01 - 1	TEST-PIT-3	97482	18.3443	-	7471B	PPB	02 Dec 2020 14:46:11	U	SMPL
L4911-01LX5 - 1		1956	0.3661	-	7471B	PPB	02 Dec 2020 14:48:27	U	SMPL
L4911-01A - 1		32495	6.1136	-	7471B	PPB	02 Dec 2020 14:50:46	U	SMPL
L4913-01DLX5 - 1		19767	3.7182	-	7471B	PPB	02 Dec 2020 14:55:57	U	SMPL
CCV21 - 1	CCV21	27337	5.1429	-	7471B	PPB	02 Dec 2020 14:58:14	U	SMPL
CCB21 - 1	CCB21	97	0.0162	-	7471B	PPB	02 Dec 2020 15:00:31	U	SMPL