


LB112276

7471B

INSTRUMENT ID: CV1

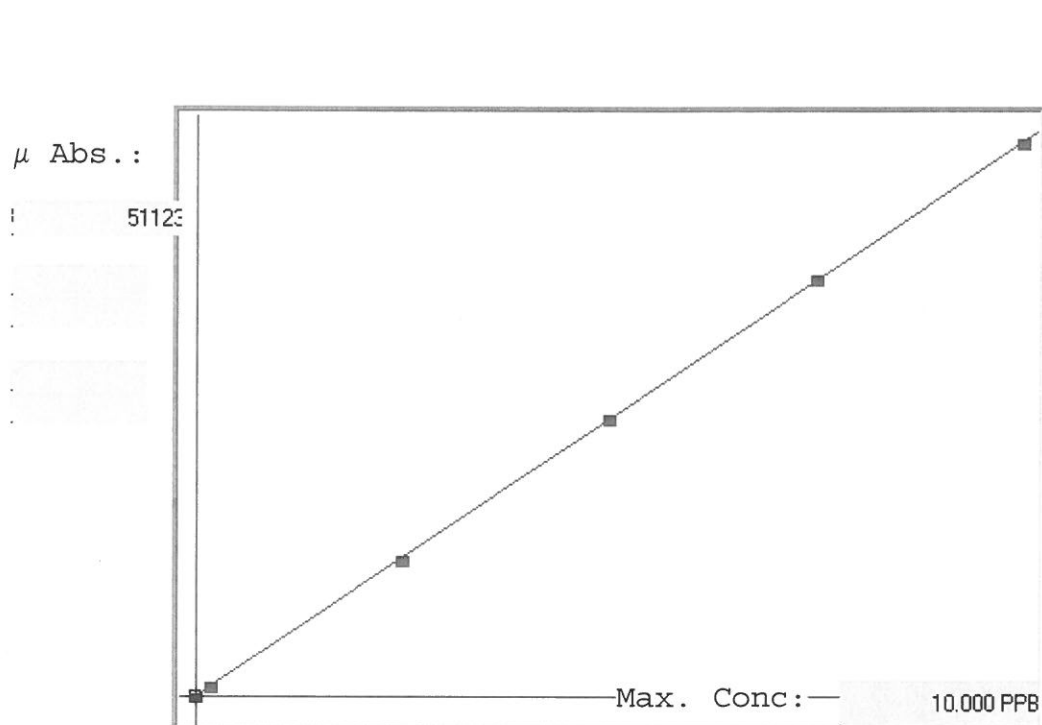

Linear

A= 0.0000e+000

B= 1.9499e-004

C= 1.1252e-003

Rho= 0.9999778

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.013	0.013	61	0.000	61				
0.2	0.200	0.189	-0.011	965	0.0 %	965				
2.5	2.500	2.479	-0.021	12710	0.0 %	12710				
5.0	5.000	5.004	0.004	25659	0.0 %	25659				
7.5	7.500	7.544	0.044	38686	0.0 %	38686				
10.0	10.000	9.970	-0.030	51123	0.0 %	51123				

LB112276 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Dec 2020 15:52:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	61	-	0.0000	7471B	PPB	08 Dec 2020 15:55:00	S	Std
0.2 - 1	50.2	965	-	0.2000	7471B	PPB	08 Dec 2020 15:57:18	S	Std
2.5 - 1	52.5	12710	-	2.5000	7471B	PPB	08 Dec 2020 15:59:35	S	Std
5.0 - 1	55	25659	-	5.0000	7471B	PPB	08 Dec 2020 16:01:52	S	Std
7.5 - 1	57.5	38686	-	7.5000	7471B	PPB	08 Dec 2020 16:04:08	S	Std
10.0 - 1	510	51123	-	10.0000	7471B	PPB	08 Dec 2020 16:06:24	S	Std
ICV32 - 1	ICV32	19744	3.8510	-	7471B	PPB	08 Dec 2020 16:09:09	U	SMPL
ICB32 - 1	ICB32	-80	-0.0145	-	7471B	PPB	08 Dec 2020 16:11:24	U	SMPL
CCV42 - 1	CCV42	26017	5.0741	-	7471B	PPB	08 Dec 2020 16:13:39	U	SMPL
CCB42 - 1	CCB42	-80	-0.0145	-	7471B	PPB	08 Dec 2020 16:15:54	U	SMPL
CRA - 1	CRA	949	0.1862	-	7471B	PPB	08 Dec 2020 16:18:09	U	SMPL
HighStd - 1	HighStd	50929	9.9317	-	7471B	PPB	08 Dec 2020 16:20:24	U	SMPL
ChkStd - 1	ChkStd	36529	7.1238	-	7471B	PPB	08 Dec 2020 16:22:39	U	SMPL
PB133468BL - 1	PBS	-114	-0.0211	-	7471B	PPB	08 Dec 2020 16:24:56	U	SMPL
PB133468BS - 1	LCSS	20098	3.9200	-	7471B	PPB	08 Dec 2020 16:27:12	U	SMPL
L4965-01 - 1	CRT012	61927	12.0762	-	7471B	PPB	08 Dec 2020 16:29:29	U	SMPL
L4965-01DUP - 1	CRT012DUP	66229	12.9150	-	7471B	PPB	08 Dec 2020 16:34:31	U	SMPL
L4965-01MS - 1	CRT012MS	83169	16.2181	-	7471B	PPB	08 Dec 2020 16:39:23	U	SMPL
L4965-01MSD - 1	CRT012MSD	80991	15.7934	-	7471B	PPB	08 Dec 2020 16:46:50	U	SMPL
L4965-06 - 1	CRT002	10290	2.0076	-	7471B	PPB	08 Dec 2020 16:49:05	U	SMPL
CCV43 - 1	CCV43	25934	5.0579	-	7471B	PPB	08 Dec 2020 16:51:22	U	SMPL
CCB43 - 1	CCB43	-68	-0.0121	-	7471B	PPB	08 Dec 2020 16:53:37	U	SMPL
L4965-11 - 1	CRT014	41996	8.1898	-	7471B	PPB	08 Dec 2020 16:55:53	U	SMPL
L4966-01 - 1	239995	27900	5.4413	-	7471B	PPB	08 Dec 2020 16:58:08	U	SMPL
L4967-01 - 1	TR-05-120720	584	0.1150	-	7471B	PPB	08 Dec 2020 17:00:25	U	SMPL
L4968-02 - 1	HSD-SOIL	580	0.1142	-	7471B	PPB	08 Dec 2020 17:02:41	U	SMPL
L4969-01 - 1	NORTH-BRANFORD-01	443	0.0875	-	7471B	PPB	08 Dec 2020 17:04:57	U	SMPL
L4969-02 - 1	NORTH-BRANFORD-02	257	0.0512	-	7471B	PPB	08 Dec 2020 17:07:13	U	SMPL
L4969-03 - 1	NORTH-BRANFORD-03	182	0.0366	-	7471B	PPB	08 Dec 2020 17:09:29	U	SMPL
L4970-01 - 1	4S2-A-D-COMP	1575	0.3082	-	7471B	PPB	08 Dec 2020 17:11:46	U	SMPL
L4970-12 - 1	4S1-A-D-COMP	1350	0.2644	-	7471B	PPB	08 Dec 2020 17:14:03	U	SMPL
L4971-01 - 1	5S1-A-D-COMP	2757	0.5387	-	7471B	PPB	08 Dec 2020 17:16:19	U	SMPL
CCV44 - 1	CCV44	26406	5.1500	-	7471B	PPB	08 Dec 2020 17:18:34	U	SMPL
CCB44 - 1	CCB44	-47	-0.0080	-	7471B	PPB	08 Dec 2020 17:20:50	U	SMPL
L4971-12 - 1	5S2-A-D-COMP	1694	0.3314	-	7471B	PPB	08 Dec 2020 17:23:06	U	SMPL
L4965-01LX5 - 1		12249	2.3895	-	7471B	PPB	08 Dec 2020 17:25:21	U	SMPL
L4965-01A - 1		84840	16.5439	-	7471B	PPB	08 Dec 2020 17:27:37	U	SMPL
L4965-01DLX5 - 1		12120	2.3644	-	7471B	PPB	08 Dec 2020 17:29:53	U	SMPL
L4965-01DUPDLX5 - 1		13229	2.5806	-	7471B	PPB	08 Dec 2020 17:32:11	U	SMPL
L4965-01MSDLX5 - 1		17144	3.3440	-	7471B	PPB	08 Dec 2020 17:34:27	U	SMPL
L4965-01MSDDLX5 - 1		16729	3.2631	-	7471B	PPB	08 Dec 2020 17:36:43	U	SMPL
L4965-01LDLX25 - 1		2506	0.4898	-	7471B	PPB	08 Dec 2020 17:39:00	U	SMPL
L4965-01ADLX5 - 1		15850	3.0917	-	7471B	PPB	08 Dec 2020 17:41:17	U	SMPL
CCV45 - 1	CCV45	26474	5.1632	-	7471B	PPB	08 Dec 2020 17:43:33	U	SMPL
CCB45 - 1	CCB45	-54	-0.0094	-	7471B	PPB	08 Dec 2020 17:45:49	U	SMPL