


LB112280

7470A

INSTRUMENT 1D: CV1

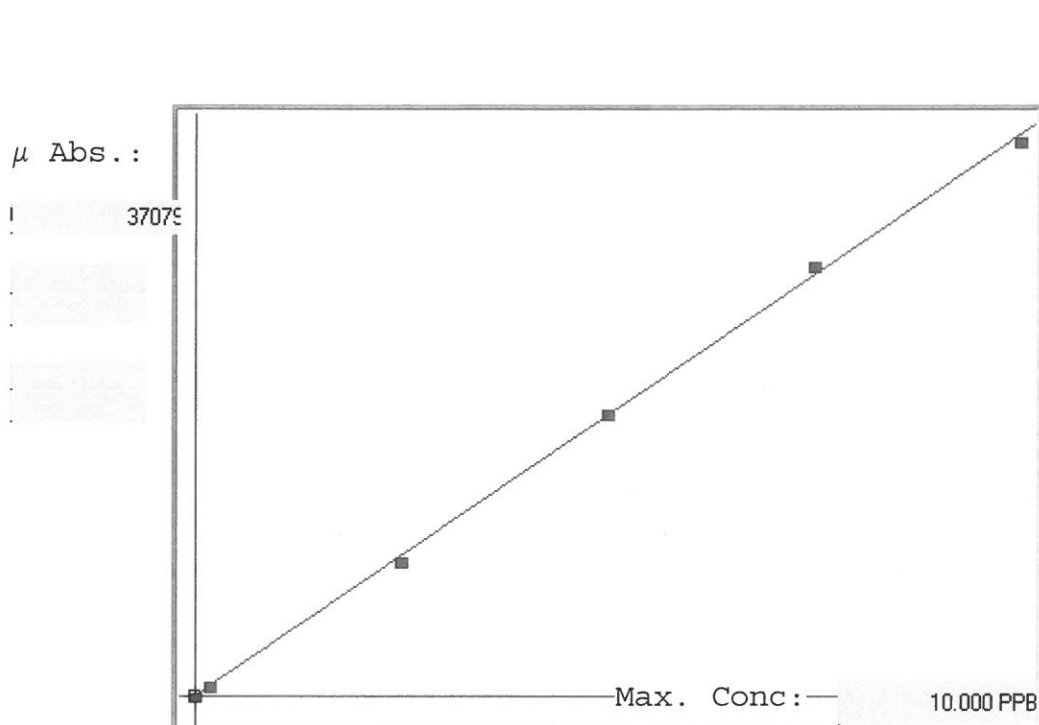

Linear

A= 0.0000e+000

B= 2.6615e-004

C= 3.9125e-003

Rho= 0.9996842

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.012	0.012	30	0.000	30				
0.2	0.200	0.192	-0.008	708	0.0 %	708				
2.5	2.500	2.428	-0.072	9108	0.0 %	9108				
5.0	5.000	5.024	0.024	18861	0.0 %	18861				
7.5	7.500	7.671	0.171	28809	0.0 %	28809				
10.0	10.000	9.873	-0.127	37079	0.0 %	37079				

LB112280 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 09 Dec 2020 12:23:12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	30	-	0.0000	7470A	PPB	09 Dec 2020 12:25:16	S	Std
0.2 - 1	50.2	708	-	0.2000	7470A	PPB	09 Dec 2020 12:27:33	S	Std
2.5 - 1	52.5	9108	-	2.5000	7470A	PPB	09 Dec 2020 12:29:50	S	Std
5.0 - 1	55	18861	-	5.0000	7470A	PPB	09 Dec 2020 12:32:07	S	Std
7.5 - 1	57.5	28809	-	7.5000	7470A	PPB	09 Dec 2020 12:34:23	S	Std
10.0 - 1	510	37079	-	10.0000	7470A	PPB	09 Dec 2020 12:44:23	S	Std
ICV33 - 1	ICV33	13573	3.6164	-	7470A	PPB	09 Dec 2020 12:47:03	U	SMPL
ICB33 - 1	ICB33	-62	-0.0126	-	7470A	PPB	09 Dec 2020 12:49:17	U	SMPL
CCV46 - 1	CCV46	18728	4.9884	-	7470A	PPB	09 Dec 2020 12:51:32	U	SMPL
CCB46 - 1	CCB46	-64	-0.0131	-	7470A	PPB	09 Dec 2020 12:53:47	U	SMPL
CRA - 1	CRA	694	0.1886	-	7470A	PPB	09 Dec 2020 12:56:02	U	SMPL
HighStd - 1	HighStd	36173	9.6314	-	7470A	PPB	09 Dec 2020 12:58:17	U	SMPL
ChkStd - 1	ChkStd	26232	6.9856	-	7470A	PPB	09 Dec 2020 13:03:10	U	SMPL
PB133492BL - 1	PBW	-111	-0.0256	-	7470A	PPB	09 Dec 2020 13:05:25	U	SMPL
PB133492BS - 1	LCSW	15860	4.2251	-	7470A	PPB	09 Dec 2020 13:07:41	U	SMPL
L4969-04 - 1	NORTH-BRANFORD-01	306	0.0854	-	7470A	PPB	09 Dec 2020 13:12:40	U	SMPL
L4969-04DUP - 1	NORTH-BRANFORD-01DUP	362	0.1003	-	7470A	PPB	09 Dec 2020 13:20:10	U	SMPL
L4969-04MS - 1	NORTH-BRANFORD-01MS	15174	4.0425	-	7470A	PPB	09 Dec 2020 13:22:26	U	SMPL
L4969-04MSD - 1	NORTH-BRANFORD-01MSD	15320	4.0813	-	7470A	PPB	09 Dec 2020 13:24:43	U	SMPL
L4969-05 - 1	NORTH-BRANFORD-02	31	0.0122	-	7470A	PPB	09 Dec 2020 13:26:58	U	SMPL
CCV47 - 1	CCV47	18796	5.0065	-	7470A	PPB	09 Dec 2020 13:29:14	U	SMPL
CCB47 - 1	CCB47	-14	0.0002	-	7470A	PPB	09 Dec 2020 13:31:29	U	SMPL
L4969-06 - 1	NORTH-BRANFORD-03	188	0.0539	-	7470A	PPB	09 Dec 2020 13:33:44	U	SMPL
PB133492TB - 1	PB133447TB	12	0.0071	-	7470A	PPB	09 Dec 2020 13:36:02	U	SMPL
L4969-04LX5 - 1		112	0.0337	-	7470A	PPB	09 Dec 2020 13:38:18	U	SMPL
L4969-04A - 1		15364	4.0931	-	7470A	PPB	09 Dec 2020 13:40:34	U	SMPL
CCV48 - 1	CCV48	18861	5.0238	-	7470A	PPB	09 Dec 2020 13:42:50	U	SMPL
CCB48 - 1	CCB48	-25	-0.0027	-	7470A	PPB	09 Dec 2020 13:45:06	U	SMPL