

LB 112324


SEAM01.0

INSTRUMENT ID: CV2

MB
12/24/20

SFAM01.1

Linear

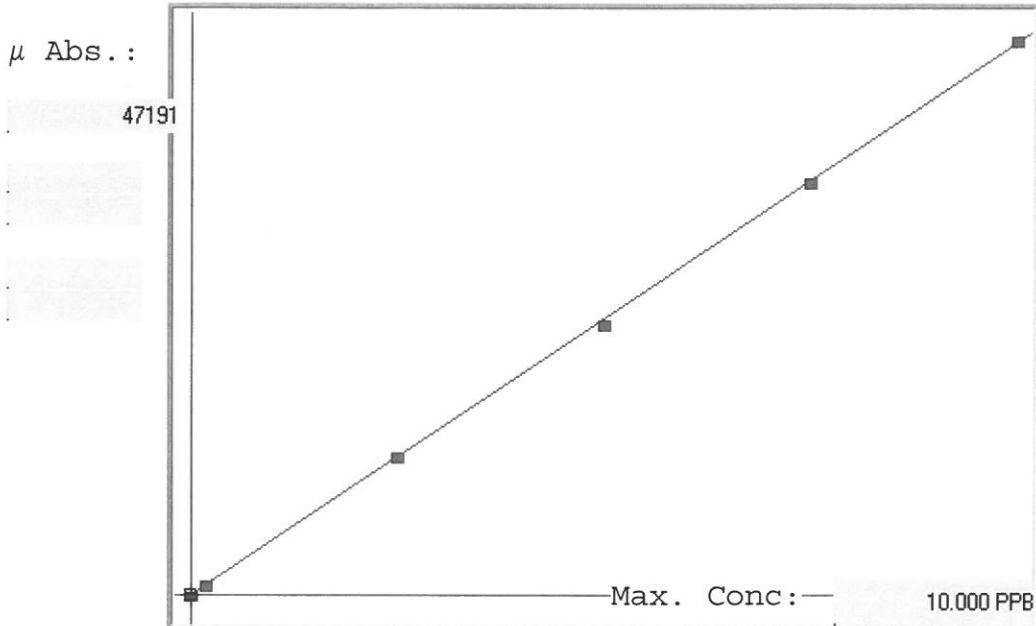

A= 0.0000e+000

B= 2.1266e-004

C= 2.0046e-003

Rho= 0.9999522

Accept=Accepted

*hope
y=mx+cept*

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.013	0.013	52	0.000	52					-
0.05	0.050					244					5
0.20	0.200	0.209	0.009	973	0.0 %	973					1
2.50	2.500	2.525	0.025	11862	0.0 %	11862					-1
5.00	5.000	4.926	-0.074	23156	0.0 %	23156					0
7.50	7.500	7.489	-0.011	35206	0.0 %	35206					0
10.0	10.000	10.038	0.038	47191	0.0 %	47191					0

LB112324
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	52	-		0 SFAM01.0	PPB	12/11/2020 13:39	Std
	0.2 S0.2	973	-		0.2 SFAM01.0	PPB	12/11/2020 13:41	Std
	2.5 S2.5	11862	-		2.5 SFAM01.0	PPB	12/11/2020 13:43	Std
	5 S5	23156	-		5 SFAM01.0	PPB	12/11/2020 13:45	Std
	7.5 S7.5	35206	-		7.5 SFAM01.0	PPB	12/11/2020 13:48	Std
	10 S10	47191	-		10 SFAM01.0	PPB	12/11/2020 13:50	Std
ICV	ICV	18472	3.9303 -		SFAM01.0	PPB	12/11/2020 13:53	SMPL
ICB	ICB	-17	-0.0016 -		SFAM01.0	PPB	12/11/2020 13:55	SMPL
CCV063	CCV063	23148	4.9248 -		SFAM01.0	PPB	12/11/2020 13:57	SMPL
CCB063	CCB063	-26	-0.0035 -		SFAM01.0	PPB	12/11/2020 13:59	SMPL
PB133542BL	PBS542	15	0.0052 -		SFAM01.0	PPB	12/11/2020 14:02	SMPL
L4956-19	X2R75	29354	6.2446 -		SFAM01.0	PPB	12/11/2020 14:06	SMPL
L4956-20	X2R75D	30423	6.4719 -		SFAM01.0	PPB	12/11/2020 14:11	SMPL
L4956-21	X2R75S	40548	8.6251 -		SFAM01.0	PPB	12/11/2020 14:13	SMPL
CCV064	CCV064	23069	4.908 -		SFAM01.0	PPB	12/11/2020 14:18	SMPL
CCB064	CCB064	-36	-0.0057 -		SFAM01.0	PPB	12/11/2020 14:20	SMPL