

LB112413

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

12/17/2020 13:05

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.990	0.0	0.090	
ICB1	-0.018	0.0	0.001	
CCV1	244.861	0.0	0.229	
CCB1	0.042	0.0	0.001	
PD1323667BL	-0.021	0.0	0.001	
L5125-02	-0.144	0.0	0.000	
L5125-02DUP	0.099	0.0	0.001	
L5125-04	0.056	0.0	0.001	
L5125-06	-0.159	0.0	0.000	
CCV2	256.523	0.0	0.240	
CCB2	0.198	0.0	0.001	

N	11
Mean	54.311
SD	101.2560
CV%	186.44

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

12/17/2020 12:36


Test Total CN

Accepted 12/17/2020 12:36

Factor 1073
Bias 0.001

Coeff. of det. 0.999950

Errors

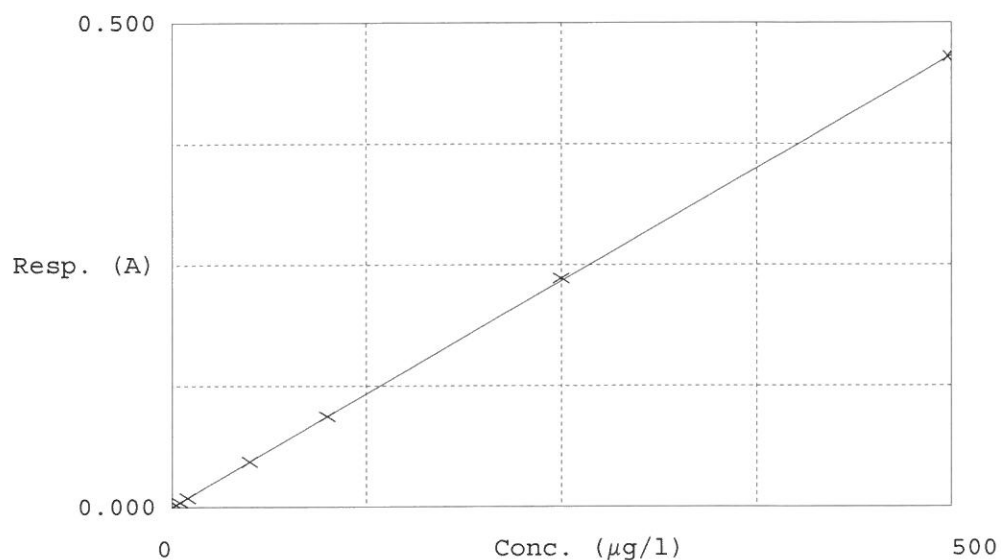

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	-0.3559	0.0000	
2	5.0PPBCN	0.005	4.4871	5.0000	
3	10PPBCN	0.010	9.6552	10.0000	
4	50PPBCN	0.047	49.7455	50.0000	
5	100PPBCN	0.094	100.0301	100.0000	
6	250PPBCN	0.236	252.8131	250.0000	
7	500PPBCN	0.465	498.6249	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Dec 17 11:50:10 2020

Thu Dec 17 13:03:28 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	-0.3559	µg/l	12/17/2020 11:50:10
5.OPPBCN	A	Reactive CN	P	4.4871	µg/l	12/17/2020 11:50:11
10PPBCN	A	Reactive CN	P	9.6552	µg/l	12/17/2020 11:50:12
50PPBCN	A	Reactive CN	P	49.7455	µg/l	12/17/2020 11:50:13
100PPBCN	A	Reactive CN	P	100.0301	µg/l	12/17/2020 11:50:14
250PPBCN	A	Reactive CN	P	252.8131	µg/l	12/17/2020 11:50:15
500PPBCN	A	Reactive CN	P	498.6249	µg/l	12/17/2020 11:50:16
ICV1	S	Reactive CN	P	95.9903	µg/l	12/17/2020 13:00:05
ICB1	S	Reactive CN	P	-0.0184	µg/l	12/17/2020 13:00:06
CCV1	S	Reactive CN	P	244.8605	µg/l	12/17/2020 13:00:08
CCB1	S	Reactive CN	P	0.0415	µg/l	12/17/2020 13:00:09
PB1323667BL	S	Reactive CN	P	-0.0214	µg/l	12/17/2020 13:00:10
L5125-02	S	Reactive CN	P	-0.1435	µg/l	12/17/2020 13:00:11
L5125-02DUP	S	Reactive CN	P	0.0986	µg/l	12/17/2020 13:00:12
L5125-04	S	Reactive CN	P	0.0561	µg/l	12/17/2020 13:00:13
L5125-06	S	Reactive CN	P	-0.1586	µg/l	12/17/2020 13:00:14
CCV2	S	Reactive CN	P	256.5226	µg/l	12/17/2020 13:03:27
CCB2	S	Reactive CN	P	0.1981	µg/l	12/17/2020 13:03:28