


LB112422

7470A

INSTRUMENT ID: CV2

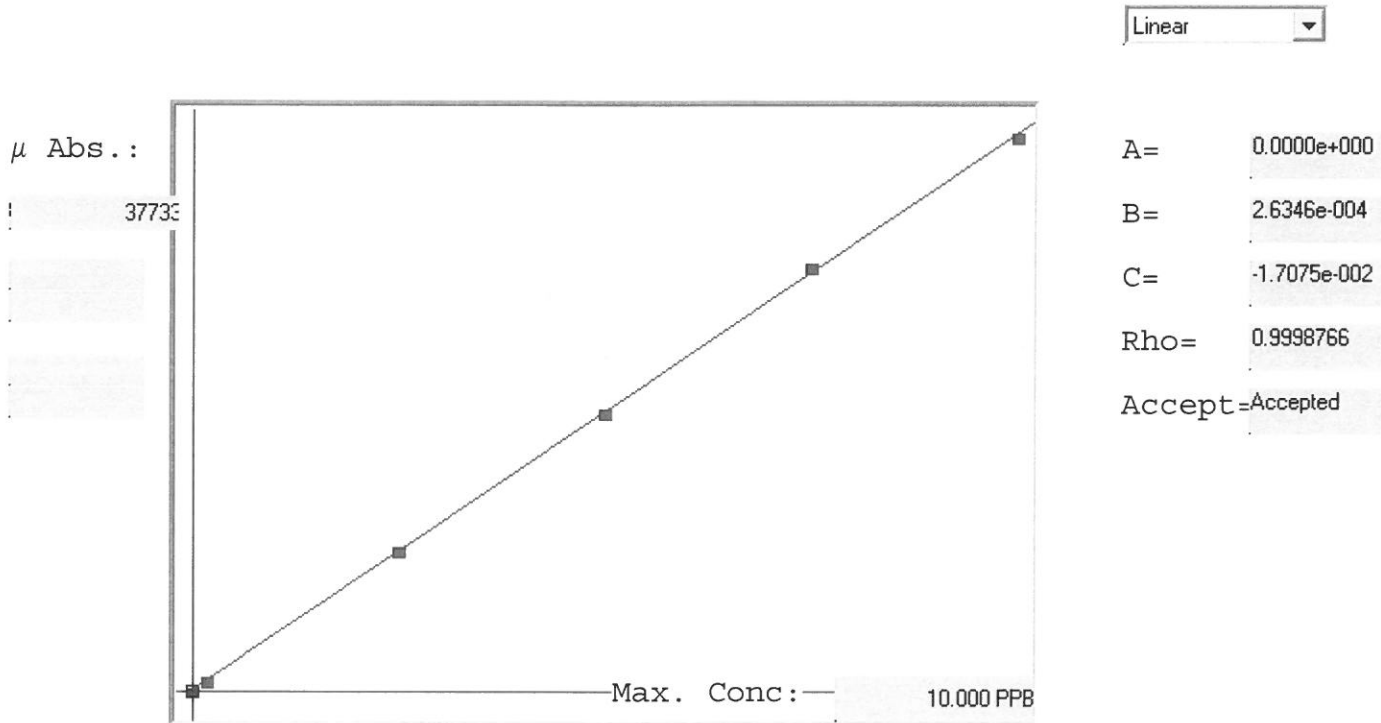

| Std ID | Conc.  | Calc. | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 |
|--------|--------|-------|--------|-------|------------|-------|-------|-------|-------|-------|
| 0.0    | 0.000  | 0.002 | 0.002  | 72    | 0.000      | 72    |       |       |       |       |
| 0.2    | 0.200  | 0.185 | -0.015 | 768   | 0.0 %      | 768   |       |       |       |       |
| 2.5    | 2.500  | 2.497 | -0.003 | 9543  | 0.0 %      | 9543  |       |       |       |       |
| 5.0    | 5.000  | 4.975 | -0.025 | 18949 | 0.0 %      | 18949 |       |       |       |       |
| 7.5    | 7.500  | 7.616 | 0.116  | 28974 | 0.0 %      | 28974 |       |       |       |       |
| 10.0   | 10.000 | 9.924 | -0.076 | 37733 | 0.0 %      | 37733 |       |       |       |       |

## LB112422 INSTRUMENT ID ; CV1

| Method: 7470A   |                         | Operator: Admin |         | Date of Analysis: 17 Dec 2020 16:02:25 |        |       |                      |      |      |
|-----------------|-------------------------|-----------------|---------|----------------------------------------|--------|-------|----------------------|------|------|
| Sample ID       | Extended ID             | µ Abs.          | Conc.   | Std Conc                               | Method | Units | Date                 | Type | Type |
| 0.0 - 1         | 50                      | 72              | -       | 0.00007470A                            | PPB    |       | 17 Dec 2020 16:04:50 | S    | Std  |
| 0.2 - 1         | 50.2                    | 768             | -       | 0.20007470A                            | PPB    |       | 17 Dec 2020 16:07:07 | S    | Std  |
| 2.5 - 1         | 52.5                    | 9543            | -       | 2.50007470A                            | PPB    |       | 17 Dec 2020 16:09:25 | S    | Std  |
| 5.0 - 1         | 55                      | 18949           | -       | 5.00007470A                            | PPB    |       | 17 Dec 2020 16:11:59 | S    | Std  |
| 7.5 - 1         | 57.5                    | 28974           | -       | 7.50007470A                            | PPB    |       | 17 Dec 2020 16:14:15 | S    | Std  |
| 10.0 - 1        | 510                     | 37733           | -       | 10.00007470A                           | PPB    |       | 17 Dec 2020 16:19:10 | S    | Std  |
| ICV46 - 1       | ICV46                   | 15183           | 3.9830  | -7470A                                 | PPB    |       | 17 Dec 2020 16:21:53 | U    | SMPL |
| ICB46 - 1       | ICB46                   | -20             | -0.0223 | -7470A                                 | PPB    |       | 17 Dec 2020 16:24:08 | U    | SMPL |
| CCV03 - 1       | CCV03                   | 18955           | 4.9768  | -7470A                                 | PPB    |       | 17 Dec 2020 16:26:23 | U    | SMPL |
| CCB03 - 1       | CCB03                   | -17             | -0.0216 | -7470A                                 | PPB    |       | 17 Dec 2020 16:28:38 | U    | SMPL |
| CRA - 1         | CRA                     | 738             | 0.1774  | -7470A                                 | PPB    |       | 17 Dec 2020 16:30:52 | U    | SMPL |
| HighStd - 1     | HighStd                 | 37926           | 9.9749  | -7470A                                 | PPB    |       | 17 Dec 2020 16:33:08 | U    | SMPL |
| ChkStd - 1      | ChkStd                  | 26300           | 6.9119  | -7470A                                 | PPB    |       | 17 Dec 2020 16:35:23 | U    | SMPL |
| PB133675BL - 1  | PBW                     | -70             | -0.0355 | -7470A                                 | PPB    |       | 17 Dec 2020 16:37:39 | U    | SMPL |
| PB133675BS - 1  | LCSW                    | 14449           | 3.7897  | -7470A                                 | PPB    |       | 17 Dec 2020 16:39:55 | U    | SMPL |
| L5139-01 - 1    | BPOW3-3-20201215        | -36             | -0.0266 | -7470A                                 | PPB    |       | 17 Dec 2020 16:42:12 | U    | SMPL |
| L5139-02 - 1    | BPOW3-4-20201215        | 19              | -0.0121 | -7470A                                 | PPB    |       | 17 Dec 2020 16:44:28 | U    | SMPL |
| L5139-03 - 1    | RE115D2-20201215        | 28              | -0.0097 | -7470A                                 | PPB    |       | 17 Dec 2020 16:46:45 | U    | SMPL |
| L5140-01 - 1    | GROUNDWATER-SAMPLE-1    | 198             | 0.0351  | -7470A                                 | PPB    |       | 17 Dec 2020 16:49:02 | U    | SMPL |
| L5140-01DUP - 1 | GROUNDWATER-SAMPLE-1DUP | 190             | 0.0330  | -7470A                                 | PPB    |       | 17 Dec 2020 16:51:17 | U    | SMPL |
| CCV04 - 1       | CCV04                   | 18824           | 4.9423  | -7470A                                 | PPB    |       | 17 Dec 2020 16:53:32 | U    | SMPL |
| CCB04 - 1       | CCB04                   | -38             | -0.0271 | -7470A                                 | PPB    |       | 17 Dec 2020 16:55:48 | U    | SMPL |
| L5140-01MS - 1  | GROUNDWATER-SAMPLE-1MS  | 15408           | 4.0423  | -7470A                                 | PPB    |       | 17 Dec 2020 16:58:04 | U    | SMPL |
| L5140-01MSD - 1 | GROUNDWATER-SAMPLE-1MSD | 15094           | 3.9596  | -7470A                                 | PPB    |       | 17 Dec 2020 17:00:19 | U    | SMPL |
| L5140-01LX5 - 1 |                         | -2              | -0.0176 | -7470A                                 | PPB    |       | 17 Dec 2020 17:02:35 | U    | SMPL |
| L5140-01A - 1   |                         | 15237           | 3.9973  | -7470A                                 | PPB    |       | 17 Dec 2020 17:04:50 | U    | SMPL |
| CCV05 - 1       | CCV05                   | 19040           | 4.9992  | -7470A                                 | PPB    |       | 17 Dec 2020 17:07:06 | U    | SMPL |
| CCB05 - 1       | CCB05                   | -17             | -0.0216 | -7470A                                 | PPB    |       | 17 Dec 2020 17:09:23 | U    | SMPL |