


LB112433

245.1

INSTRUMENT ID: CV2

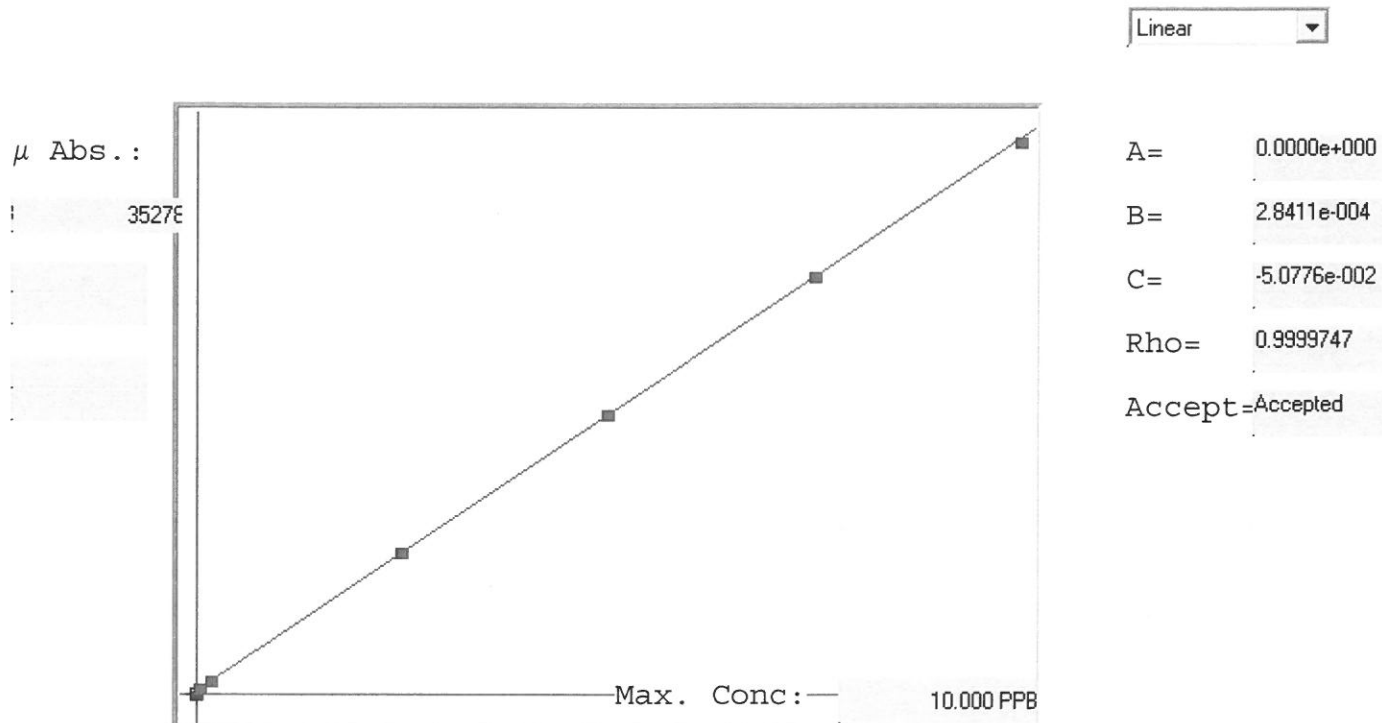

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.050	-0.050	3	0.000	3				
0.05	0.050	0.055	0.005	373	0.0 %	373	0			
0.2	0.200	0.211	0.011	921	0.0 %	921				
2.5	2.500	2.532	0.032	9090	0.0 %	9090				
5.0	5.000	5.013	0.013	17823	0.0 %	17823				
7.5	7.500	7.517	0.017	26636	0.0 %	26636				
10.0	10.000	9.972	-0.028	35278	0.0 %	35278				

LB112433 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 18 Dec 2020 11:44:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	3	-	0.0000	245.1	PPB	18 Dec 2020 12:04:45	S	Std
0.05 - 1	50.05	373	-	0.0500	245.1	PPB	18 Dec 2020 12:07:03	S	Std
0.2 - 1	50.2	921	-	0.2000	245.1	PPB	18 Dec 2020 12:09:20	S	Std
2.5 - 1	52.5	9090	-	2.5000	245.1	PPB	18 Dec 2020 12:11:37	S	Std
5.0 - 1	55	17823	-	5.0000	245.1	PPB	18 Dec 2020 12:13:53	S	Std
7.5 - 1	57.5	26636	-	7.5000	245.1	PPB	18 Dec 2020 12:18:45	S	Std
10.0 - 1	50	35278	-	10.0000	245.1	PPB	18 Dec 2020 12:31:57	S	Std
ICV47 - 1	ICV47	13669	3.8328	-245.1		PPB	18 Dec 2020 12:40:12	U	SMPL
ICB47 - 1	ICB47	4	-0.0496	-245.1		PPB	18 Dec 2020 12:42:27	U	SMPL
CCV06 - 1	CCV06	18115	5.0959	-245.1		PPB	18 Dec 2020 12:44:42	U	SMPL
CCB06 - 1	CCB06	20	-0.0451	-245.1		PPB	18 Dec 2020 12:46:57	U	SMPL
CRA - 1	CRA	357	0.0507	-245.1		PPB	18 Dec 2020 12:49:12	U	SMPL
HighStd - 1	HighStd	35513	10.0389	-245.1		PPB	18 Dec 2020 12:51:28	U	SMPL
ChkStd - 1	ChkStd	24946	7.0367	-245.1		PPB	18 Dec 2020 12:53:43	U	SMPL
PB133682BL - 1	PBW	85	-0.0266	-245.1		PPB	18 Dec 2020 12:58:39	U	SMPL
PB133682BS - 1	LCSW	12742	3.5694	-245.1		PPB	18 Dec 2020 13:00:54	U	SMPL
L4981-01 - 1	EFFLUENT-DAY1-METALS	313	0.0382	-245.1		PPB	18 Dec 2020 13:03:11	U	SMPL
L5028-07 - 1	14B-(1-4)-COMP	635	0.1296	-245.1		PPB	18 Dec 2020 13:05:27	U	SMPL
L5051-07 - 1	14B-(1-4)-COMP	487	0.0876	-245.1		PPB	18 Dec 2020 13:07:44	U	SMPL
L5051-07DUP - 1	14B-(1-4)-COMP DUP	422	0.0691	-245.1		PPB	18 Dec 2020 13:10:01	U	SMPL
L5051-07MS - 1	14B-(1-4)-COMPMS	14675	4.1186	-245.1		PPB	18 Dec 2020 13:12:16	U	SMPL
CCV07 - 1	CCV07	17808	5.0087	-245.1		PPB	18 Dec 2020 13:14:32	U	SMPL
CCB07 - 1	CCB07	9	-0.0482	-245.1		PPB	18 Dec 2020 13:16:47	U	SMPL
L5051-07MSD - 1	14B-(1-4)-COMPMSD	14809	4.1567	-245.1		PPB	18 Dec 2020 13:19:03	U	SMPL
L5051-07LX5 - 1		57	-0.0346	-245.1		PPB	18 Dec 2020 13:21:18	U	SMPL
L5051-07A - 1		14525	4.0760	-245.1		PPB	18 Dec 2020 13:23:33	U	SMPL
CCV08 - 1	CCV08	17638	4.9604	-245.1		PPB	18 Dec 2020 13:25:49	U	SMPL
CCB08 - 1	CCB08	11	-0.0477	-245.1		PPB	18 Dec 2020 13:28:05	U	SMPL