


LB112489

245.1

INSTRUMENT ID: CV1

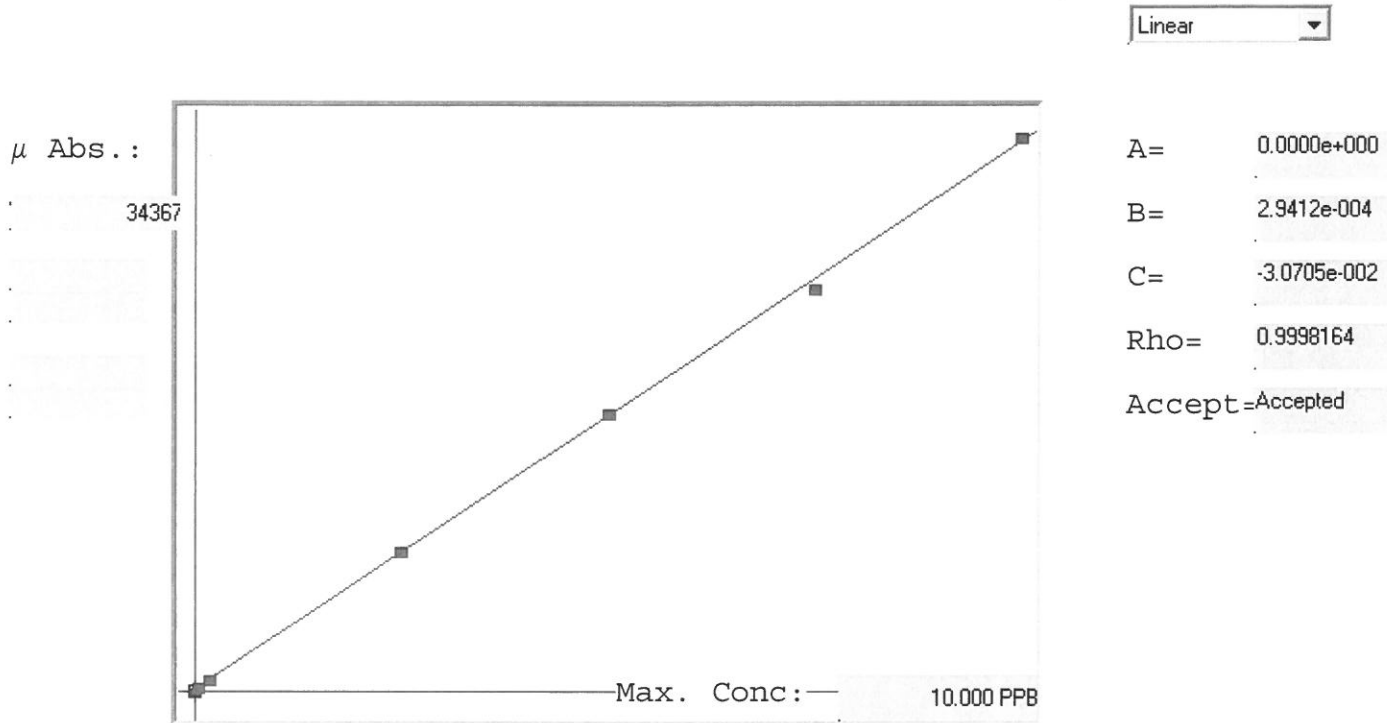

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	69	0.000	69				
0.05	0.050	0.047	-0.003	265	0.0 %	265	0			
0.2	0.200	0.192	-0.008	756	0.0 %	756				
2.5	2.500	2.556	0.056	8794	0.0 %	8794				
5.0	5.000	5.044	0.044	17253	0.0 %	17253				
7.5	7.500	7.344	-0.156	25075	0.0 %	25075				
10.0	10.000	10.077	0.077	34367	0.0 %	34367				

LB112489 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 22 Dec 2020 11:58:13

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	69	-	0.0000245.1	PPB	22 Dec 2020 12:22:00	S	Std
0.05 - 1	50.05	265	-	0.0500245.1	PPB	22 Dec 2020 12:24:17	S	Std
0.2 - 1	50.2	756	-	0.2000245.1	PPB	22 Dec 2020 12:26:34	S	Std
2.5 - 1	52.5	8794	-	2.5000245.1	PPB	22 Dec 2020 12:28:51	S	Std
5.0 - 1	55	17253	-	5.0000245.1	PPB	22 Dec 2020 12:31:08	S	Std
7.5 - 1	57.5	25075	-	7.5000245.1	PPB	22 Dec 2020 12:33:24	S	Std
10.0 - 1	510	34367	-	10.0000245.1	PPB	22 Dec 2020 12:40:55	S	Std
ICV50 - 1	ICV50	13933	4.0673	-245.1	PPB	22 Dec 2020 12:46:07	U	SMPL
ICB50 - 1	ICB50	57	-0.0139	-245.1	PPB	22 Dec 2020 12:48:22	U	SMPL
CCV19 - 1	CCV19	17540	5.1282	-245.1	PPB	22 Dec 2020 12:50:38	U	SMPL
CCB19 - 1	CCB19	44	-0.0178	-245.1	PPB	22 Dec 2020 12:52:53	U	SMPL
CRA - 1	CRA	250	0.0428	-245.1	PPB	22 Dec 2020 12:55:08	U	SMPL
HighStd - 1	HighStd	35012	10.2672	-245.1	PPB	22 Dec 2020 12:57:23	U	SMPL
ChkStd - 1	ChkStd	24435	7.1562	-245.1	PPB	22 Dec 2020 12:59:39	U	SMPL
PB133754BL - 1	PBW	59	-0.0134	-245.1	PPB	22 Dec 2020 13:04:27	U	SMPL
PB133754BS - 1	LCSW	14271	4.1667	-245.1	PPB	22 Dec 2020 13:06:43	U	SMPL
L5153-07 - 1	14B-(1-4)-COMP	1915	0.5325	-245.1	PPB	22 Dec 2020 13:14:06	U	SMPL
L5153-07DUP - 1	14B-(1-4)-COMPDUP	1852	0.5140	-245.1	PPB	22 Dec 2020 13:16:23	U	SMPL
L5153-07MS - 1	14B-(1-4)-COMPMS	13513	3.9438	-245.1	PPB	22 Dec 2020 13:18:40	U	SMPL
L5153-07MSD - 1	14B-(1-4)-COMPMSD	13647	3.9832	-245.1	PPB	22 Dec 2020 13:23:30	U	SMPL
L5174-07 - 1	14B-(1-4)-COMP	624	0.1528	-245.1	PPB	22 Dec 2020 13:25:45	U	SMPL
CCV20 - 1	CCV20	17682	5.1700	-245.1	PPB	22 Dec 2020 13:28:01	U	SMPL
CCB20 - 1	CCB20	106	0.0005	-245.1	PPB	22 Dec 2020 13:30:16	U	SMPL
L5153-07LX5 - 1		484	0.1117	-245.1	PPB	22 Dec 2020 13:32:32	U	SMPL
L5153-07A - 1		15468	4.5188	-245.1	PPB	22 Dec 2020 13:34:47	U	SMPL
CCV21 - 1	CCV21	17566	5.1359	-245.1	PPB	22 Dec 2020 13:37:03	U	SMPL
CCB21 - 1	CCB21	-11	-0.0339	-245.1	PPB	22 Dec 2020 13:39:19	U	SMPL