


LB112536

7471B

INSTRUMENT 1A: CV1

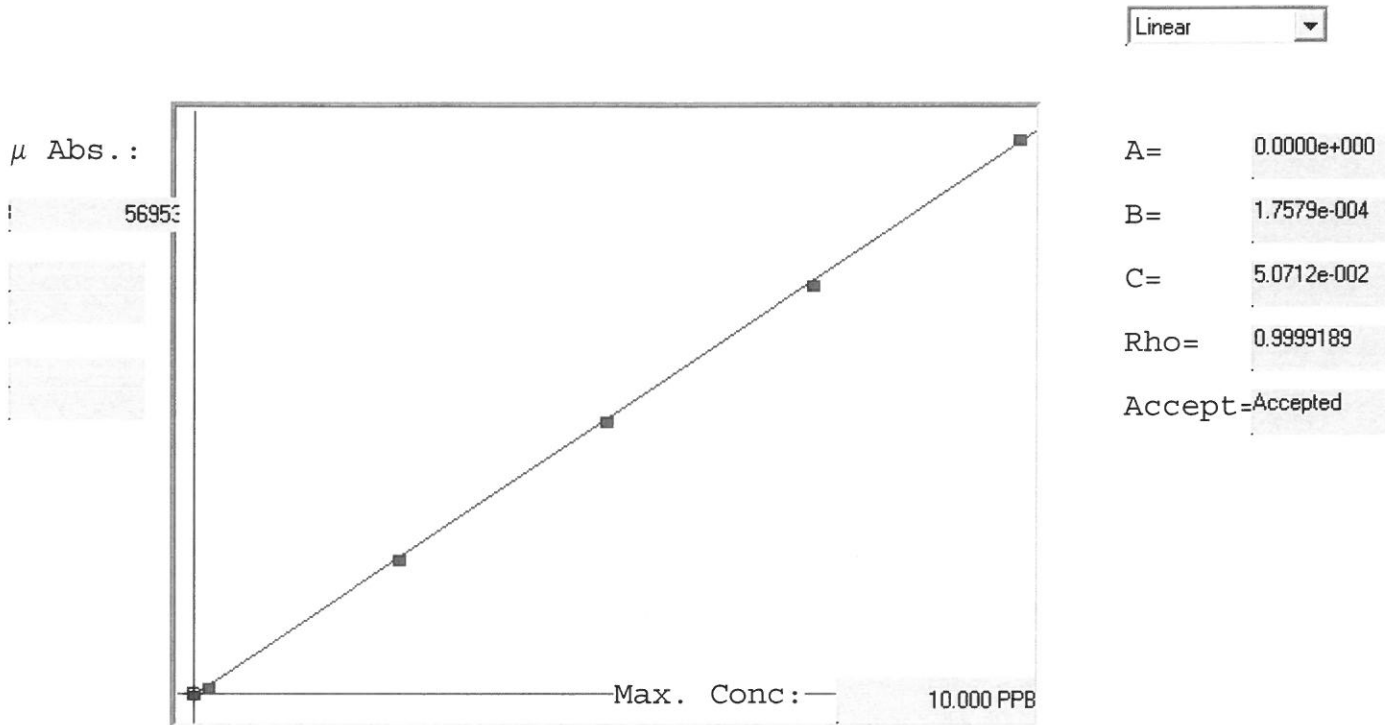

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.063	0.063	69	0.000	69				
0.2	0.200	0.175	-0.025	706	0.0 %	706				
2.5	2.500	2.491	-0.009	13882	0.0 %	13882				
5.0	5.000	4.971	-0.029	27988	0.0 %	27988				
7.5	7.500	7.438	-0.062	42024	0.0 %	42024				
10.0	10.000	10.062	0.062	56953	0.0 %	56953				

LB112536 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 24 Dec 2020 15:19:10

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	69	-	0.00007471B	PPB	24 Dec 2020 15:21:53	S	Std
0.2 - 1	50.2	706	-	0.20007471B	PPB	24 Dec 2020 15:24:10	S	Std
2.5 - 1	52.5	13882	-	2.50007471B	PPB	24 Dec 2020 15:26:28	S	Std
5.0 - 1	55	27988	-	5.00007471B	PPB	24 Dec 2020 15:28:45	S	Std
7.5 - 1	57.5	42024	-	7.50007471B	PPB	24 Dec 2020 15:31:01	S	Std
10.0 - 1	510	56953	-	10.00007471B	PPB	24 Dec 2020 15:33:17	S	Std
ICV53 - 1	ICV53	21301	3.7952	-7471B	PPB	24 Dec 2020 15:36:58	U	SMPL
ICB53 - 1	ICB53	-16	0.0479	-7471B	PPB	24 Dec 2020 15:39:13	U	SMPL
CCV33 - 1	CCV33	28199	5.0078	-7471B	PPB	24 Dec 2020 15:41:28	U	SMPL
CCB33 - 1	CCB33	-19	0.0474	-7471B	PPB	24 Dec 2020 15:43:43	U	SMPL
CRA - 1	CRA	689	0.1718	-7471B	PPB	24 Dec 2020 15:45:58	U	SMPL
HighStd - 1	HighStd	56820	10.0391	-7471B	PPB	24 Dec 2020 15:48:13	U	SMPL
ChkStd - 1	ChkStd	39999	7.0821	-7471B	PPB	24 Dec 2020 15:50:29	U	SMPL
PB133793BL - 1	PBS	-50	0.0419	-7471B	PPB	24 Dec 2020 15:52:46	U	SMPL
PB133793BS - 1	LCSS	19629	3.5013	-7471B	PPB	24 Dec 2020 15:55:03	U	SMPL
L5186-01 - 1	SP-138KV-YARD	2630	0.5130	-7471B	PPB	24 Dec 2020 15:57:20	U	SMPL
L5188-01 - 1	NB-08-122220	1262	0.2726	-7471B	PPB	24 Dec 2020 15:59:37	U	SMPL
L5189-01 - 1	22	115812	20.4093	-7471B	PPB	24 Dec 2020 16:01:54	U	SMPL
L5189-06 - 1	09	6973	1.2765	-7471B	PPB	24 Dec 2020 16:04:11	U	SMPL
L5189-06DUP - 1	09DUP	6001	1.1056	-7471B	PPB	24 Dec 2020 16:06:29	U	SMPL
CCV34 - 1	CCV34	27900	4.9553	-7471B	PPB	24 Dec 2020 16:08:45	U	SMPL
CCB34 - 1	CCB34	-34	0.0447	-7471B	PPB	24 Dec 2020 16:11:00	U	SMPL
L5189-06MS - 1	09MS	26453	4.7009	-7471B	PPB	24 Dec 2020 16:16:02	U	SMPL
L5189-06MSD - 1	09MSD	26966	4.7911	-7471B	PPB	24 Dec 2020 16:18:17	U	SMPL
L5189-11 - 1	18	2329	0.4601	-7471B	PPB	24 Dec 2020 16:20:32	U	SMPL
L5189-16 - 1	08	90331	15.9300	-7471B	PPB	24 Dec 2020 16:22:48	U	SMPL
L5190-01 - 1	OK-01-122220	1061	0.2372	-7471B	PPB	24 Dec 2020 16:25:04	U	SMPL
L5192-01 - 1	CL-02-122220	3229	0.6183	-7471B	PPB	24 Dec 2020 16:27:23	U	SMPL
L5197-01 - 1	EO-01-122320	1409	0.2984	-7471B	PPB	24 Dec 2020 16:29:40	U	SMPL
L5198-01 - 1	EO-03-122320	3097	0.5951	-7471B	PPB	24 Dec 2020 16:31:58	U	SMPL
L5199-01 - 1	OR-03-122320	1342	0.2866	-7471B	PPB	24 Dec 2020 16:34:15	U	SMPL
L5200-01 - 1	BIN-4-122320	1346	0.2873	-7471B	PPB	24 Dec 2020 16:36:31	U	SMPL
CCV35 - 1	CCV35	27662	4.9134	-7471B	PPB	24 Dec 2020 16:38:47	U	SMPL
CCB35 - 1	CCB35	-63	0.0396	-7471B	PPB	24 Dec 2020 16:41:02	U	SMPL
L5201-01 - 1	HD-02-122320	1885	0.3821	-7471B	PPB	24 Dec 2020 16:43:19	U	SMPL
L5207-01 - 1	SP-1	5182	0.9617	-7471B	PPB	24 Dec 2020 16:45:34	U	SMPL
L5189-06LX5 - 1		1306	0.2803	-7471B	PPB	24 Dec 2020 16:47:50	U	SMPL
L5189-06A - 1		29195	5.1829	-7471B	PPB	24 Dec 2020 16:50:06	U	SMPL
L5189-01DLX5 - 1		22836	4.0651	-7471B	PPB	24 Dec 2020 16:52:22	U	SMPL
L5189-16DLX5 - 1		17958	3.2075	-7471B	PPB	24 Dec 2020 16:54:39	U	SMPL
CCV36 - 1	CCV36	27669	4.9146	-7471B	PPB	24 Dec 2020 16:56:55	U	SMPL
CCB36 - 1	CCB36	-53	0.0414	-7471B	PPB	24 Dec 2020 16:59:12	U	SMPL