


LB112587

7471B

INSTRUMENT ID: CV1

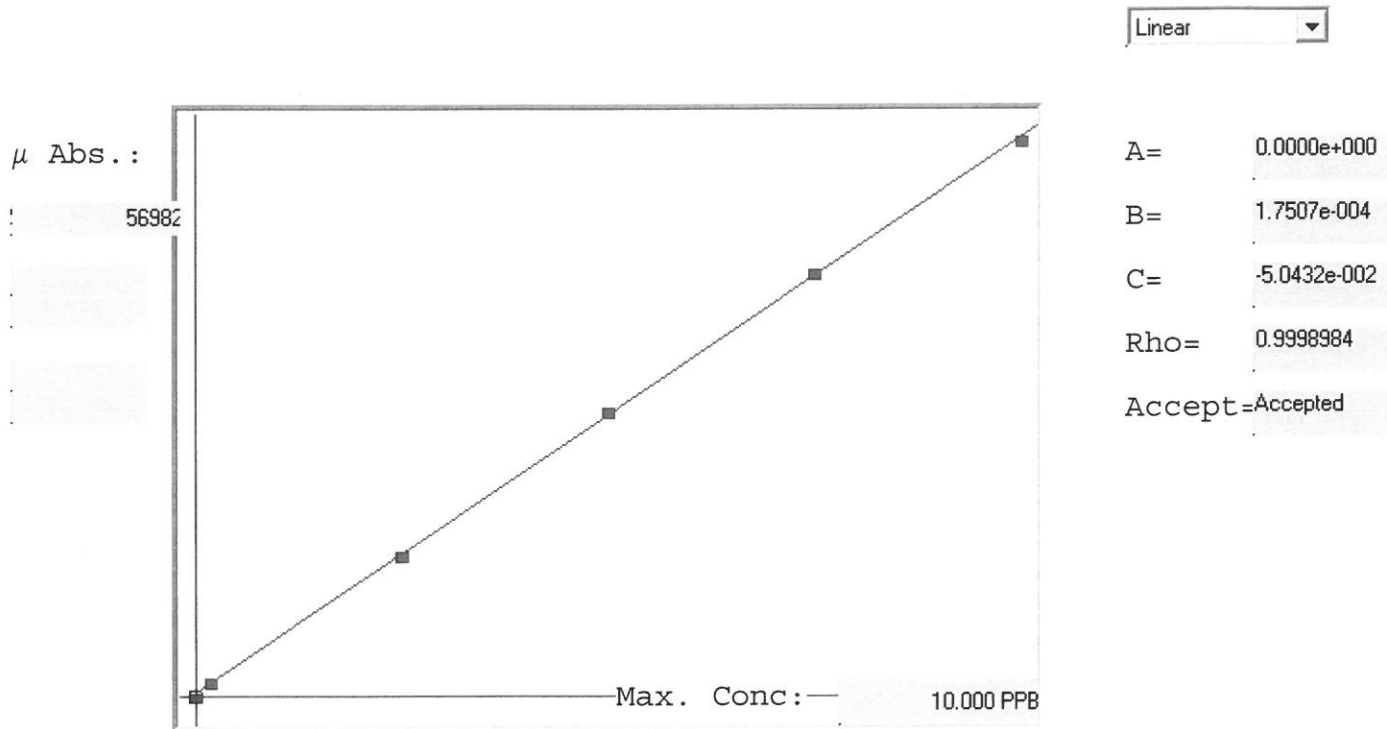

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.047	-0.047	22	0.000	22				
0.2	0.200	0.216	0.016	1522	0.0 %	1522				
2.5	2.500	2.478	-0.022	14443	0.0 %	14443				
5.0	5.000	5.069	0.069	29241	0.0 %	29241				
7.5	7.500	7.558	0.058	43461	0.0 %	43461				
10.0	10.000	9.925	-0.075	56982	0.0 %	56982				

LB112587 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 31 Dec 2020 12:04:22

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	22	-	0.00007471B	PPB	31 Dec 2020 13:30:14	S	Std
0.2 - 1	50.2	1522	-	0.20007471B	PPB	31 Dec 2020 13:32:31	S	Std
2.5 - 1	52.5	14443	-	2.50007471B	PPB	31 Dec 2020 13:34:49	S	Std
5.0 - 1	55	29241	-	5.00007471B	PPB	31 Dec 2020 13:37:07	S	Std
7.5 - 1	57.5	43461	-	7.50007471B	PPB	31 Dec 2020 13:39:23	S	Std
10.0 - 1	510	56982	-	10.00007471B	PPB	31 Dec 2020 13:41:39	S	Std
ICV57 - 1	ICV57	22326	3.8582	-7471B	PPB	31 Dec 2020 13:44:22	U	SMPL
ICB57 - 1	ICB57	339	0.0089	-7471B	PPB	31 Dec 2020 13:46:37	U	SMPL
CCV58 - 1	CCV58	29304	5.0798	-7471B	PPB	31 Dec 2020 13:48:52	U	SMPL
CCB58 - 1	CCB58	460	0.0301	-7471B	PPB	31 Dec 2020 13:51:08	U	SMPL
CRA - 1	CRA	1505	0.2130	-7471B	PPB	31 Dec 2020 13:53:24	U	SMPL
HighStd - 1	HighStd	57388	9.9965	-7471B	PPB	31 Dec 2020 13:55:39	U	SMPL
ChkStd - 1	ChkStd	40326	7.0094	-7471B	PPB	31 Dec 2020 14:00:28	U	SMPL
PB133882BL - 1	PBS	658	0.0648	-7471B	PPB	31 Dec 2020 14:05:18	U	SMPL
PB133882BS - 1	LCSS	19551	3.3724	-7471B	PPB	31 Dec 2020 14:07:34	U	SMPL
L5235-01 - 1	TR-05-122920	12590	2.1537	-7471B	PPB	31 Dec 2020 14:09:50	U	SMPL
L5235-01DUP - 1	TR-05-122920DUP	14464	2.4818	-7471B	PPB	31 Dec 2020 14:12:06	U	SMPL
L5235-01MS - 1	TR-05-122920MS	34905	6.0604	-7471B	PPB	31 Dec 2020 14:16:59	U	SMPL
L5235-01MSD - 1	TR-05-122920MSD	33177	5.7579	-7471B	PPB	31 Dec 2020 14:19:16	U	SMPL
L5242-01 - 1	SAMPLE-1(494+26)	1388	0.1926	-7471B	PPB	31 Dec 2020 14:21:32	U	SMPL
CCV59 - 1	CCV59	29407	5.0978	-7471B	PPB	31 Dec 2020 14:23:47	U	SMPL
CCB59 - 1	CCB59	433	0.0254	-7471B	PPB	31 Dec 2020 14:26:02	U	SMPL
L5242-03 - 1	SAMPLE-2(484+26)	3274	0.5227	-7471B	PPB	31 Dec 2020 14:28:18	U	SMPL
L5242-05 - 1	SAMPLE-3(474+26)	7956	1.3424	-7471B	PPB	31 Dec 2020 14:30:33	U	SMPL
L5242-07 - 1	SAMPLE-4(464+26)	2512	0.3893	-7471B	PPB	31 Dec 2020 14:32:49	U	SMPL
L5242-09 - 1	SAMPLE-5(454+26)	4410	0.7216	-7471B	PPB	31 Dec 2020 14:35:05	U	SMPL
L5242-11 - 1	SAMPLE-6(444+26)	3036	0.4811	-7471B	PPB	31 Dec 2020 14:37:21	U	SMPL
L5242-13 - 1	SAMPLE-7(434+26)	4056	0.6597	-7471B	PPB	31 Dec 2020 14:39:37	U	SMPL
L5244-01 - 1	HR-01-123020	6943	1.1651	-7471B	PPB	31 Dec 2020 14:41:53	U	SMPL
L5235-01LX5 - 1		2484	0.3844	-7471B	PPB	31 Dec 2020 14:44:11	U	SMPL
L5235-01A - 1		34970	6.0718	-7471B	PPB	31 Dec 2020 14:46:28	U	SMPL
CCV60 - 1	CCV60	29742	5.1565	-7471B	PPB	31 Dec 2020 14:48:43	U	SMPL
CCB60 - 1	CCB60	553	0.0464	-7471B	PPB	31 Dec 2020 14:51:00	U	SMPL