


LB112646

SFAM01.1

INSTRUMENT ID: EV1

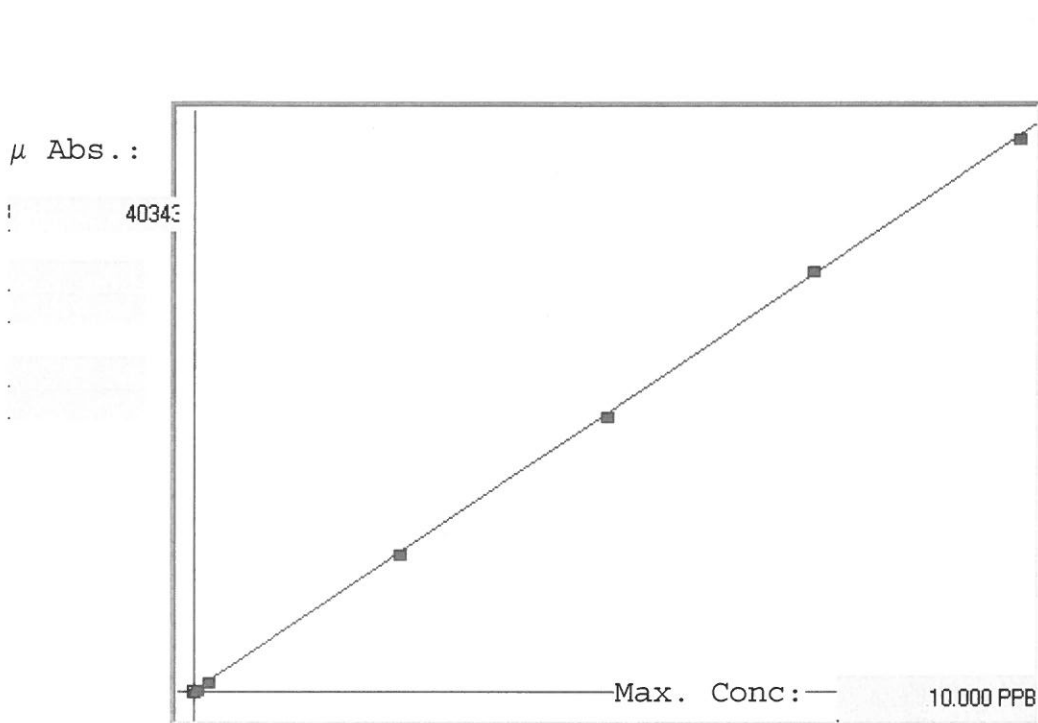

Linear

A= 0.0000e+000

B= 2.4668e-004

C= -3.6328e-003

Rho= 0.9999233

Accept=Accepted

slope
y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.011	0.011	58	0.000	58					4
0.05	0.050	0.052	0.002	226	0.0 %	226					-4
0.20	0.200	0.192	-0.008	794	0.0 %	794					0
2.50	2.500	2.491	-0.009	10114	0.0 %	10114					-1
5.00	5.000	4.956	-0.044	20105	0.0 %	20105					1
7.50	7.500	7.600	0.100	30822	0.0 %	30822					-1
10.0	10.000	9.948	-0.052	40343	0.0 %	40343					

LB112646
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S00	58	-		0 SFAM01.1	PPB	1/6/2021 12:35	Std
	0.05 S01	226	-	0.05	SFAM01.1	PPB	1/6/2021 12:37	Std
	0.2 S02	794	-	0.2	SFAM01.1	PPB	1/6/2021 12:40	Std
	2.5 S03	10114	-	2.5	SFAM01.1	PPB	1/6/2021 12:42	Std
	5 S04	20105	-	5	SFAM01.1	PPB	1/6/2021 12:44	Std
	7.5 S05	30822	-	7.5	SFAM01.1	PPB	1/6/2021 12:52	Std
	10 S06	40343	-	10	SFAM01.1	PPB	1/6/2021 12:54	Std
ICV007	ICV007	15995	3.942 -		SFAM01.1	PPB	1/6/2021 12:57	SMPL
ICB007	ICB007	-27	-0.0103 -		SFAM01.1	PPB	1/6/2021 12:59	SMPL
CCV077	CCV077	20031	4.9376 -		SFAM01.1	PPB	1/6/2021 13:02	SMPL
CCB077	CCB077	-36	-0.0125 -		SFAM01.1	PPB	1/6/2021 13:04	SMPL
PB133945BL	PBW945	11	-0.0009 -		SFAM01.1	PPB	1/6/2021 13:06	SMPL
L5214-02	MDL-WATER-QT1-2021-02	227	0.0524 -		SFAM01.1	PPB	1/6/2021 13:11	SMPL
CCV078	CCV078	19918	4.9098 -		SFAM01.1	PPB	1/6/2021 13:13	SMPL
CCB078	CCB078	-15	-0.0073 -		SFAM01.1	PPB	1/6/2021 13:15	SMPL