


LB112648

7470A

INSTRUMENT ID: CV1

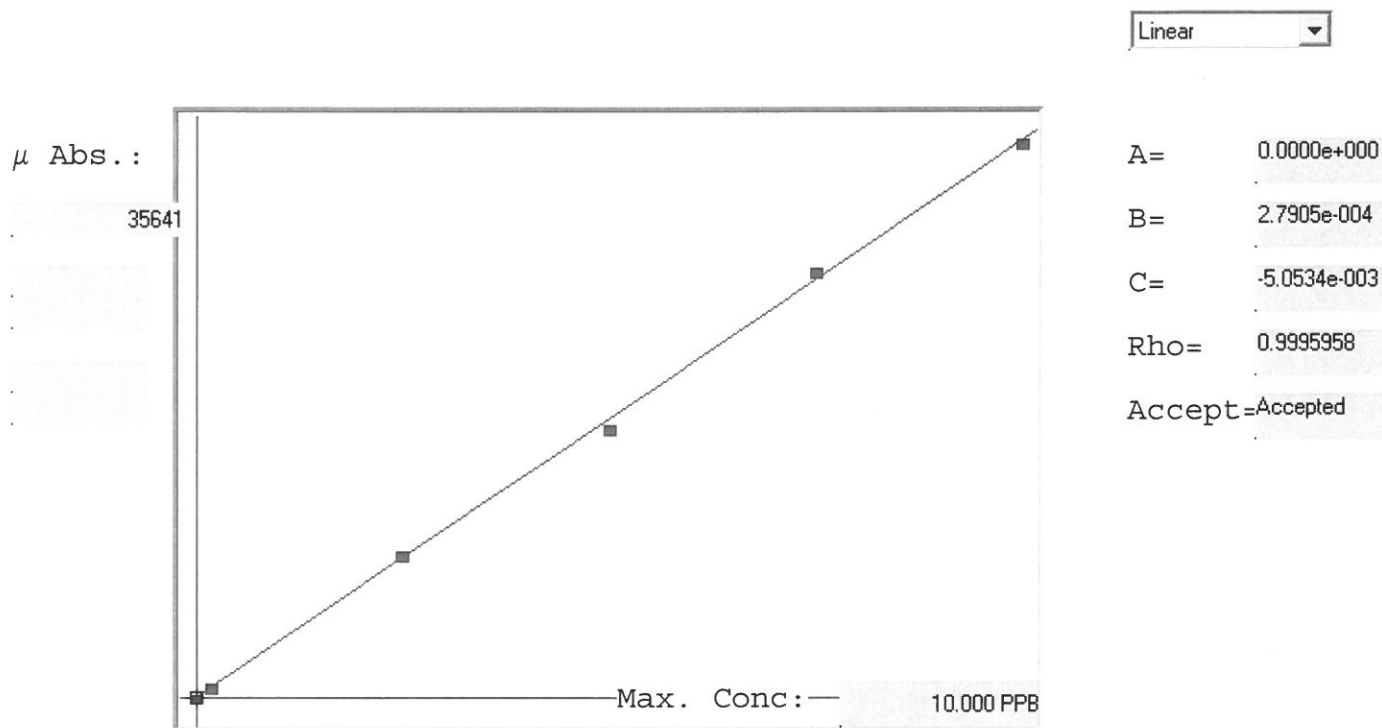

| Std ID | Conc.  | Calc. | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 |
|--------|--------|-------|--------|-------|------------|-------|-------|-------|-------|-------|
| 0.0    | 0.000  | 0.011 | 0.011  | 57    | 0.000      | 57    |       |       |       |       |
| 0.2    | 0.200  | 0.191 | -0.009 | 701   | 0.0 %      | 701   |       |       |       |       |
| 2.5    | 2.500  | 2.568 | 0.068  | 9222  | 0.0 %      | 9222  |       |       |       |       |
| 5.0    | 5.000  | 4.825 | -0.175 | 17310 | 0.0 %      | 17310 |       |       |       |       |
| 7.5    | 7.500  | 7.665 | 0.165  | 27485 | 0.0 %      | 27485 |       |       |       |       |
| 10.0   | 10.000 | 9.940 | -0.060 | 35641 | 0.0 %      | 35641 |       |       |       |       |

## LB112648 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Jan 2021 14:10:58

| Sample ID       | Extended ID | $\mu$ Abs. | Conc.   | Std Conc | Method | Units | Date                 | Type | Type |
|-----------------|-------------|------------|---------|----------|--------|-------|----------------------|------|------|
| 0.0 - 1         | 50          | 57         | -       | 0.0000   | 7470A  | PPB   | 06 Jan 2021 14:12:11 | S    | Std  |
| 0.2 - 1         | 50.2        | 701        | -       | 0.2000   | 7470A  | PPB   | 06 Jan 2021 14:14:29 | S    | Std  |
| 2.5 - 1         | 52.1        | 9222       | -       | 2.5000   | 7470A  | PPB   | 06 Jan 2021 14:16:47 | S    | Std  |
| 5.0 - 1         | 55          | 17310      | -       | 5.0000   | 7470A  | PPB   | 06 Jan 2021 14:19:03 | S    | Std  |
| 7.5 - 1         | 57.5        | 27485      | -       | 7.5000   | 7470A  | PPB   | 06 Jan 2021 14:21:20 | S    | Std  |
| 10.0 - 1        | 510         | 35641      | -       | 10.0000  | 7470A  | PPB   | 06 Jan 2021 14:23:36 | S    | Std  |
| ICV61 - 1       | ICV61       | 15049      | 4.1943  | -        | 7470A  | PPB   | 06 Jan 2021 14:27:56 | U    | SMPL |
| ICB61 - 1       | ICB61       | -42        | -0.0168 | -        | 7470A  | PPB   | 06 Jan 2021 14:30:11 | U    | SMPL |
| CCV79 - 1       | CCV79       | 18390      | 5.1266  | -        | 7470A  | PPB   | 06 Jan 2021 14:32:26 | U    | SMPL |
| CCB79 - 1       | CCB79       | -41        | -0.0165 | -        | 7470A  | PPB   | 06 Jan 2021 14:34:42 | U    | SMPL |
| CRA - 1         | CRA         | 681        | 0.1850  | -        | 7470A  | PPB   | 06 Jan 2021 14:36:57 | U    | SMPL |
| HighStd - 1     | HighStd     | 37387      | 10.4277 | -        | 7470A  | PPB   | 06 Jan 2021 14:39:12 | U    | SMPL |
| ChkStd - 1      | ChkStd      | 24953      | 6.9580  | -        | 7470A  | PPB   | 06 Jan 2021 14:41:28 | U    | SMPL |
| PB133939BL - 1  | PBW         | -76        | -0.0263 | -        | 7470A  | PPB   | 06 Jan 2021 14:43:44 | U    | SMPL |
| PB133939BS - 1  | LCSW        | 14689      | 4.0939  | -        | 7470A  | PPB   | 06 Jan 2021 14:48:32 | U    | SMPL |
| M1008-17 - 1    | 375-393     | -15        | -0.0092 | -        | 7470A  | PPB   | 06 Jan 2021 14:50:47 | U    | SMPL |
| M1008-17DUP - 1 | 375-393DUP  | 5          | -0.0037 | -        | 7470A  | PPB   | 06 Jan 2021 14:53:04 | U    | SMPL |
| M1008-17MS - 1  | 375-393MS   | 14245      | 3.9700  | -        | 7470A  | PPB   | 06 Jan 2021 14:57:52 | U    | SMPL |
| M1008-17MSD - 1 | 375-393MSD  | 14014      | 3.9055  | -        | 7470A  | PPB   | 06 Jan 2021 15:00:09 | U    | SMPL |
| M1008-19 - 1    | 376-384     | 90         | 0.0201  | -        | 7470A  | PPB   | 06 Jan 2021 15:02:24 | U    | SMPL |
| CCV80 - 1       | CCV80       | 18065      | 5.0359  | -        | 7470A  | PPB   | 06 Jan 2021 15:04:39 | U    | SMPL |
| CCB80 - 1       | CCB80       | -32        | -0.0140 | -        | 7470A  | PPB   | 06 Jan 2021 15:06:55 | U    | SMPL |
| M1008-21 - 1    | 388-392     | 86         | 0.0189  | -        | 7470A  | PPB   | 06 Jan 2021 15:09:10 | U    | SMPL |
| M1010-02 - 1    | MT          | 11         | -0.0020 | -        | 7470A  | PPB   | 06 Jan 2021 15:11:26 | U    | SMPL |
| PB133940BL - 1  | PBW         | 20         | 0.0005  | -        | 7470A  | PPB   | 06 Jan 2021 15:13:41 | U    | SMPL |
| PB133940BS - 1  | LCSW        | 14466      | 4.0316  | -        | 7470A  | PPB   | 06 Jan 2021 15:15:57 | U    | SMPL |
| M1011-02 - 1    | N48967      | 32         | 0.0039  | -        | 7470A  | PPB   | 06 Jan 2021 15:18:13 | U    | SMPL |
| M1011-02DUP - 1 | N48967DUP   | 52         | 0.0095  | -        | 7470A  | PPB   | 06 Jan 2021 15:20:29 | U    | SMPL |
| M1011-02MS - 1  | N48967MS    | 14971      | 4.1726  | -        | 7470A  | PPB   | 06 Jan 2021 15:22:45 | U    | SMPL |
| M1011-02MSD - 1 | N48967MSD   | 14378      | 4.0071  | -        | 7470A  | PPB   | 06 Jan 2021 15:25:02 | U    | SMPL |
| CCV81 - 1       | CCV81       | 17435      | 4.8601  | -        | 7470A  | PPB   | 06 Jan 2021 15:27:19 | U    | SMPL |
| CCB81 - 1       | CCB81       | -60        | -0.0218 | -        | 7470A  | PPB   | 06 Jan 2021 15:29:35 | U    | SMPL |
| PB133939TB - 1  | PB133927TB  | 0          | -0.0051 | -        | 7470A  | PPB   | 06 Jan 2021 15:31:51 | U    | SMPL |
| M1008-17LX5 - 1 |             | 15         | -0.0009 | -        | 7470A  | PPB   | 06 Jan 2021 15:34:06 | U    | SMPL |
| M1008-17A - 1   |             | 13471      | 3.7540  | -        | 7470A  | PPB   | 06 Jan 2021 15:36:22 | U    | SMPL |
| M1011-02LX5 - 1 |             | -21        | -0.0109 | -        | 7470A  | PPB   | 06 Jan 2021 15:38:38 | U    | SMPL |
| M1011-02A - 1   |             | 14373      | 4.0057  | -        | 7470A  | PPB   | 06 Jan 2021 15:40:53 | U    | SMPL |
| CCV82 - 1       | CCV82       | 16805      | 4.6843  | -        | 7470A  | PPB   | 06 Jan 2021 15:43:09 | U    | SMPL |
| CCB82 - 1       | CCB82       | -39        | -0.0159 | -        | 7470A  | PPB   | 06 Jan 2021 15:45:25 | U    | SMPL |