


LB112656

7471B

INSTRUMENT ID: CV1

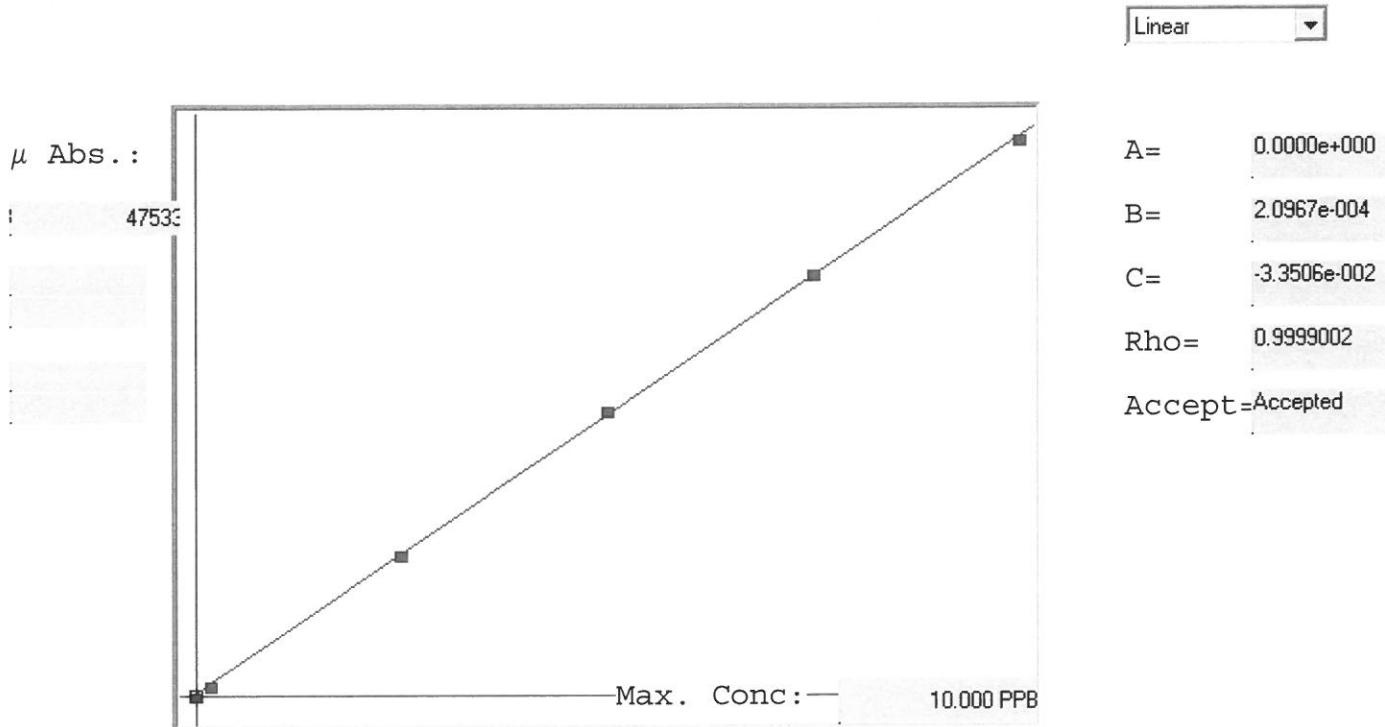

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.018	-0.018	73	0.000	73				
0.2	0.200	0.160	-0.040	925	0.0 %	925				
2.5	2.500	2.506	0.006	12113	0.0 %	12113				
5.0	5.000	5.097	0.097	24469	0.0 %	24469				
7.5	7.500	7.521	0.021	36032	0.0 %	36032				
10.0	10.000	9.933	-0.067	47533	0.0 %	47533				

LB112656 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 06 Jan 2021 16:12:40

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	73	-	0.0000	7471B	PPB	06 Jan 2021 16:14:34	S	Std
0.2 - 1	50.2	925	-	0.2000	7471B	PPB	06 Jan 2021 16:16:51	S	Std
2.5 - 1	52.5	12113	-	2.5000	7471B	PPB	06 Jan 2021 16:19:09	S	Std
5.0 - 1	53	24469	-	5.0000	7471B	PPB	06 Jan 2021 16:21:26	S	Std
7.5 - 1	57.5	36032	-	7.5000	7471B	PPB	06 Jan 2021 16:23:42	S	Std
10.0 - 1	510	47533	-	10.0000	7471B	PPB	06 Jan 2021 16:25:58	S	Std
ICV62 - 1	ICV62	18775	3.9031	-7471B	PPB	PPB	06 Jan 2021 16:28:41	U	SMPL
ICB62 - 1	ICB62	-5	-0.0346	-7471B	PPB	PPB	06 Jan 2021 16:30:56	U	SMPL
CCV83 - 1	CCV83	23827	4.9624	-7471B	PPB	PPB	06 Jan 2021 16:33:11	U	SMPL
CCB83 - 1	CCB83	-19	-0.0375	-7471B	PPB	PPB	06 Jan 2021 16:35:27	U	SMPL
CRA - 1	CRA	951	0.1659	-7471B	PPB	PPB	06 Jan 2021 16:37:42	U	SMPL
HighStd - 1	HighStd	47058	9.8334	-7471B	PPB	PPB	06 Jan 2021 16:39:57	U	SMPL
ChkStd - 1	ChkStd	32240	6.7264	-7471B	PPB	PPB	06 Jan 2021 16:42:13	U	SMPL
PB133920BL - 1	PBS	-41	-0.0421	-7471B	PPB	PPB	06 Jan 2021 16:44:29	U	SMPL
PB133920BS - 1	LCSS	16431	3.4117	-7471B	PPB	PPB	06 Jan 2021 16:46:46	U	SMPL
M1000-01 - 1	OR-02-010421	5811	1.1849	-7471B	PPB	PPB	06 Jan 2021 16:49:03	U	SMPL
M1006-01 - 1	R-LA-21-5-WC	1578	0.2974	-7471B	PPB	PPB	06 Jan 2021 16:56:13	U	SMPL
M1006-01DUP - 1	R-LA-21-5-WCDUP	1480	0.2768	-7471B	PPB	PPB	06 Jan 2021 16:58:29	U	SMPL
M1006-01MS - 1	R-LA-21-5-WCMS	17355	3.6054	-7471B	PPB	PPB	06 Jan 2021 17:00:46	U	SMPL
M1006-01MSD - 1	R-LA-21-5-WCMSD	17306	3.5951	-7471B	PPB	PPB	06 Jan 2021 17:03:01	U	SMPL
CCV84 - 1	CCV84	23259	4.8433	-7471B	PPB	PPB	06 Jan 2021 17:05:17	U	SMPL
CCB84 - 1	CCB84	-6	-0.0348	-7471B	PPB	PPB	06 Jan 2021 17:07:32	U	SMPL
M1007-01 - 1	R-LA-22-1-WC	2168	0.4211	-7471B	PPB	PPB	06 Jan 2021 17:09:48	U	SMPL
M1015-01 - 1	NB-01-010521	1143	0.2062	-7471B	PPB	PPB	06 Jan 2021 17:12:03	U	SMPL
M1006-01LX5 - 1		307	0.0309	-7471B	PPB	PPB	06 Jan 2021 17:14:19	U	SMPL
M1006-01A - 1		18523	3.8503	-7471B	PPB	PPB	06 Jan 2021 17:16:35	U	SMPL
CCV85 - 1	CCV85	23170	4.8247	-7471B	PPB	PPB	06 Jan 2021 17:18:51	U	SMPL
CCB85 - 1	CCB85	-25	-0.0387	-7471B	PPB	PPB	06 Jan 2021 17:21:07	U	SMPL