


LB112686

7471B

INSTRUMENT ID: CV1

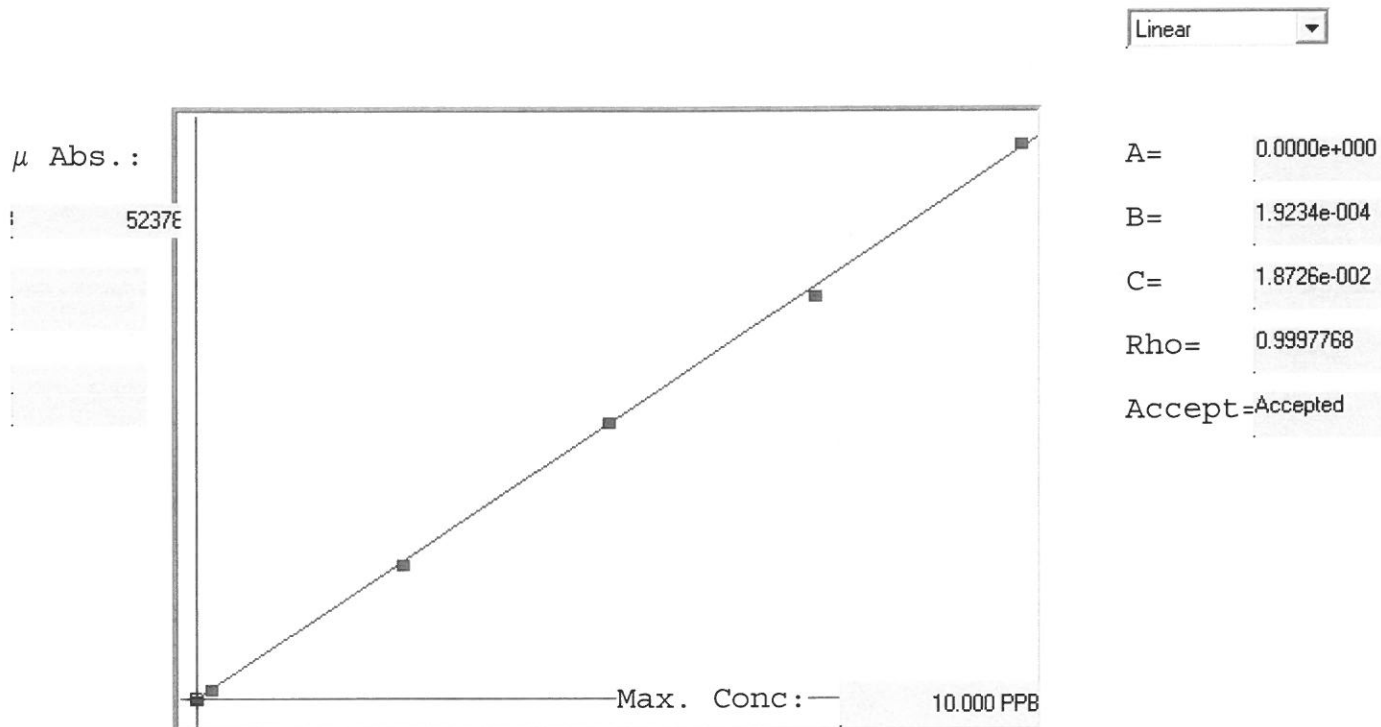

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.025	0.025	33	0.000	33				
0.2	0.200	0.220	0.020	1049	0.0 %	1049				
2.5	2.500	2.461	-0.039	12696	0.0 %	12696				
5.0	5.000	5.051	0.051	26165	0.0 %	26165				
7.5	7.500	7.350	-0.150	38115	0.0 %	38115				
10.0	10.000	10.093	0.093	52378	0.0 %	52378				

LB112686 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 08 Jan 2021 12:02:20					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	33	-	0.0000	7471B	PPB	08 Jan 2021 12:05:01	S	Std
0.2 - 1	50.2	1049	-	0.2000	7471B	PPB	08 Jan 2021 12:07:18	S	Std
2.5 - 1	52.5	12696	-	2.5000	7471B	PPB	08 Jan 2021 12:09:35	S	Std
5.0 - 1	55	26165	-	5.0000	7471B	PPB	08 Jan 2021 12:11:51	S	Std
7.5 - 1	57.5	38115	-	7.5000	7471B	PPB	08 Jan 2021 12:14:08	S	Std
10.0 - 1	510	52378	-	10.0000	7471B	PPB	08 Jan 2021 12:16:24	S	Std
ICV65 - 1	ICV65	19241	3.7195	-	7471B	PPB	08 Jan 2021 12:19:05	U	SMPL
ICB65 - 1	ICB65	-34	0.0122	-	7471B	PPB	08 Jan 2021 12:21:19	U	SMPL
CCV92 - 1	CCV92	26802	5.1737	-	7471B	PPB	08 Jan 2021 12:23:35	U	SMPL
CCB92 - 1	CCB92	-33	0.0124	-	7471B	PPB	08 Jan 2021 12:25:49	U	SMPL
CRA - 1	CRA	1043	0.2193	-	7471B	PPB	08 Jan 2021 12:28:05	U	SMPL
HighStd - 1	HighStd	52336	10.0849	-	7471B	PPB	08 Jan 2021 12:30:20	U	SMPL
ChkStd - 1	ChkStd	35259	6.8003	-	7471B	PPB	08 Jan 2021 12:32:36	U	SMPL
PB134004BL - 1	PBS	-56	0.0080	-	7471B	PPB	08 Jan 2021 12:34:53	U	SMPL
PB134004BS - 1	LCSS	18207	3.5206	-	7471B	PPB	08 Jan 2021 12:37:10	U	SMPL
M1038-10 - 1	CT-SP	1928	0.3896	-	7471B	PPB	08 Jan 2021 12:39:26	U	SMPL
M1042-02 - 1	11939	6826	1.3316	-	7471B	PPB	08 Jan 2021 12:41:43	U	SMPL
M1043-01 - 1	BALL-1	3494	0.6908	-	7471B	PPB	08 Jan 2021 12:43:59	U	SMPL
M1044-01 - 1	TP-2	844	0.1811	-	7471B	PPB	08 Jan 2021 12:46:17	U	SMPL
M1044-01DUP - 1	TP-2DUP	948	0.2011	-	7471B	PPB	08 Jan 2021 12:48:32	U	SMPL
CCV93 - 1	CCV93	26131	5.0447	-	7471B	PPB	08 Jan 2021 12:50:47	U	SMPL
CCB93 - 1	CCB93	-40	0.0110	-	7471B	PPB	08 Jan 2021 12:53:02	U	SMPL
M1044-01MS - 1	TP-2MS	18926	3.6589	-	7471B	PPB	08 Jan 2021 12:55:18	U	SMPL
M1044-01MSD - 1	TP-2MSD	18933	3.6602	-	7471B	PPB	08 Jan 2021 12:57:34	U	SMPL
M1044-03 - 1	TP-4	27051	5.2216	-	7471B	PPB	08 Jan 2021 12:59:49	U	SMPL
M1044-05 - 1	TP-6	876	0.1872	-	7471B	PPB	08 Jan 2021 13:02:05	U	SMPL
M1044-07 - 1	TP-8	7994	1.5563	-	7471B	PPB	08 Jan 2021 13:04:22	U	SMPL
M1044-09 - 1	TP-10	2957	0.5875	-	7471B	PPB	08 Jan 2021 13:06:38	U	SMPL
M1044-11 - 1	TP-11	5789	1.1322	-	7471B	PPB	08 Jan 2021 13:08:55	U	SMPL
M1044-19 - 1	TP-12	3118	0.6184	-	7471B	PPB	08 Jan 2021 13:11:12	U	SMPL
M1044-01LX5 - 1		166	0.0507	-	7471B	PPB	08 Jan 2021 13:13:29	U	SMPL
M1044-01A - 1		20668	3.9939	-	7471B	PPB	08 Jan 2021 13:15:45	U	SMPL
CCV94 - 1	CCV94	26490	5.1137	-	7471B	PPB	08 Jan 2021 13:18:00	U	SMPL
CCB94 - 1	CCB94	-44	0.0103	-	7471B	PPB	08 Jan 2021 13:20:16	U	SMPL