

Clear table


IC-1
300.0
01/11/2021
AM

ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-01-04_	1/4/21 18:42		AM/AP
STD2	0.2400	0.3550	0.3640	1.2460	0.3180	0.3700	1.8630	2021-01-04_	1/4/21 19:15		AM/AP
STD3	0.4060	0.6050	0.6140	2.0910	0.5250	0.9790	3.0800	2021-01-04_	1/4/21 19:48		AM/AP
STD4	0.8160	1.1930	1.1950	4.0200	1.0110	2.0270	6.0080	2021-01-04_	1/4/21 20:21		AM/AP
STD5	1.9130	2.9230	2.9330	9.6190	2.3930	5.2740	14.4730	2021-01-04_	1/4/21 20:54		AM/AP
STD6	3.9900	5.9800	5.8760	19.5750	4.8710	9.8350	29.5540	2021-01-04_	1/4/21 21:26		AM/AP
STD7	5.0360	7.5440	7.6180	25.4480	6.3810	12.5150	38.0220	2021-01-04_	1/4/21 21:59		AM/AP
ICV	1.8850	3.0940	2.9200	9.6530	2.4160	5.0140	14.4080	2021-01-04_	1/4/21 22:32		AM/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-01-04_	1/4/21 23:05		AM/AP
CCV	2.0300	2.8740	2.8540	9.4530	2.3500	4.8900	14.5170	2021-01-08_	1/8/21 10:14		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-01-08_	1/8/21 10:48		AM/AP
LB112696BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-01-08_	1/8/21 11:20		AM/AP
LB112696BSW	2.0510	2.9080	2.8810	9.3750	2.3860	5.0650	14.1630	2021-01-08_	1/8/21 11:53		AM/AP
M1046-01	0.3820	2050.6780	0.0000	0.9500	0.0000	0.0000	34.7500	2021-01-08_	1/8/21 12:39		AM/AP
M1046-01DUP	0.3700	2051.4150	0.0000	0.9460	0.0000	0.0000	34.5310	2021-01-08_	1/8/21 13:11		AM/AP
M1046-01MS	2.4600	1856.0470	2.8260	10.3260	2.4470	5.0060	48.5000	2021-01-08_	1/8/21 13:44		AM/AP
M1046-01MSD	2.4320	1875.3380	2.9370	10.6220	2.5360	5.3710	46.8780	2021-01-08_	1/8/21 14:49		AM/AP
M1046-01DLX50C	0.0000	2.4530	0.0000	0.0000	0.0000	0.0000	0.0000	2021-01-08_	1/8/21 15:21		AM/AP
L1062-03	0.2300	225.4870	0.0000	2.1790	0.0000	0.0000	2.7380	2021-01-08_	1/8/21 16:32		AM/AP
CCV	1.9300	2.7090	2.7750	9.3270	2.3340	5.0680	13.5250	2021-01-08_	1/8/21 17:38		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-01-08_	1/8/21 18:10		AM/AP

CALIBRATION OF COMPONENT F-

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 0.88025 \cdot A + 1.60325$
 RSD: 2.525 %
 Correlation coefficient: 0.999731

IC-1
 300.0
 01/05/2021
 AM

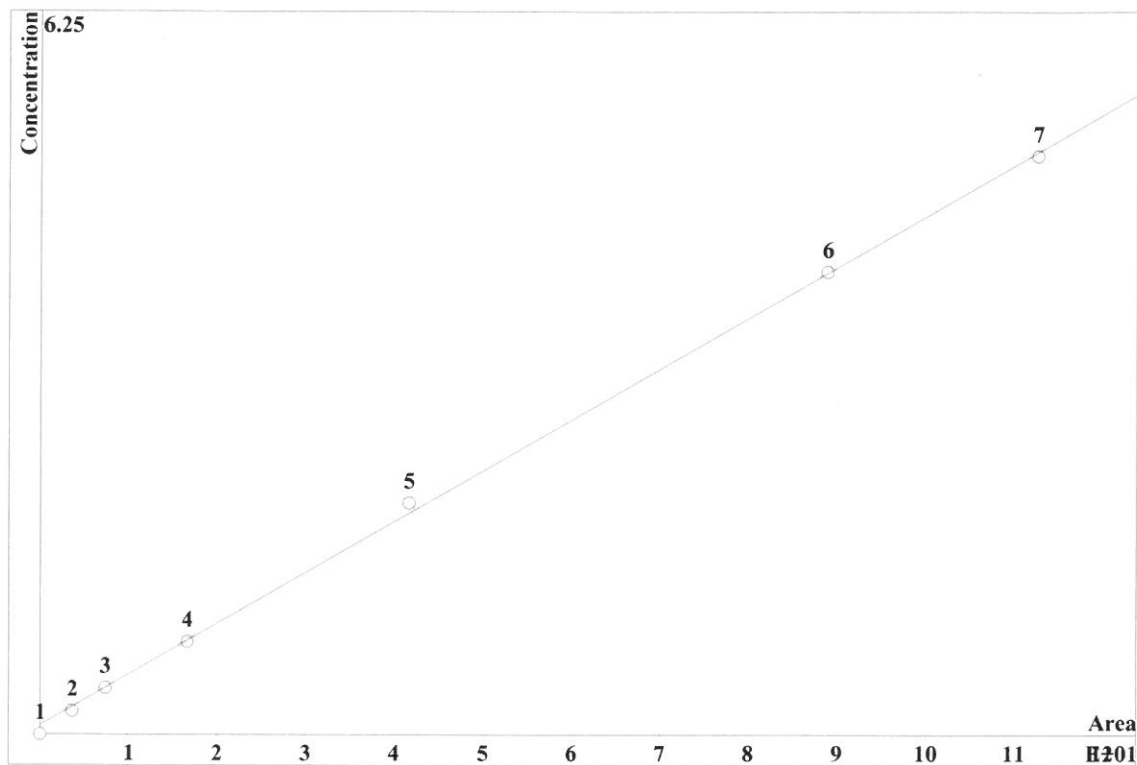

K3 = 0 K2 = 0 K1 = 0.88025 K0 = 1.60325

Base: Area

Ref.channel: Cond

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.09627	3.624	0.2	20	5.822	Yes	
3	0.1858	7.398	0.4	20	5.822	Yes	
4	0.4894	16.71	0.8	20	5.822	Yes	
5	1.175	41.64	2	20	5.822	Yes	
6	2.507	88.83	4	20	5.822	Yes	
7	3.11	112.6	5	20	5.822	Yes	

CALIBRATION OF COMPONENT CL-

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 1.31202 \cdot A + 1.4264$
 RSD: 1.725 %
 Correlation coefficient: 0.999874

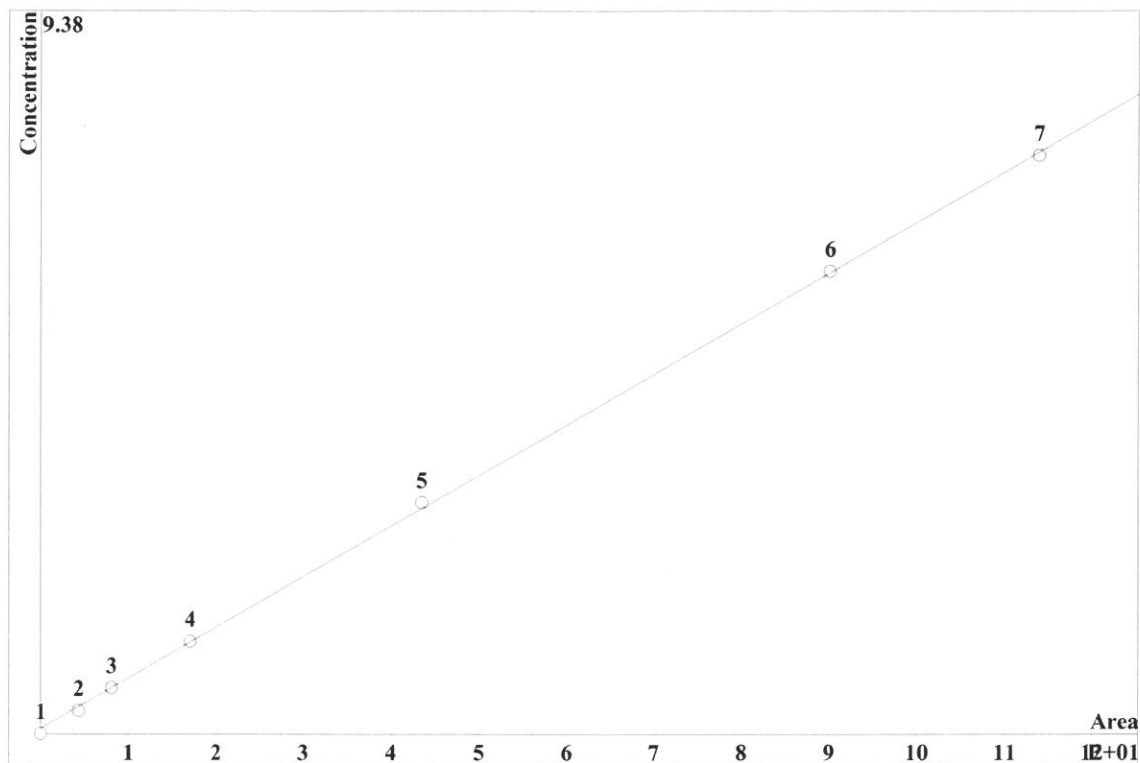


K3 = 0 K2 = 0 K1 = 1.31202 K0 = 1.4264

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.3226	4.331	0.3	20	9.31	Yes	
3	0.6113	8.137	0.6	20	9.31	Yes	
4	1.297	17.09	1.2	20	9.31	Yes	
5	3.318	43.47	3	20	9.31	Yes	
6	6.958	90.07	6	20	9.31	Yes	
7	8.989	113.9	7.5	20	9.31	Yes	

CALIBRATION OF COMPONENT NO2

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 0.587678 \cdot A + 2.15085$
 RSD: 3.152 %
 Correlation coefficient: 0.999580

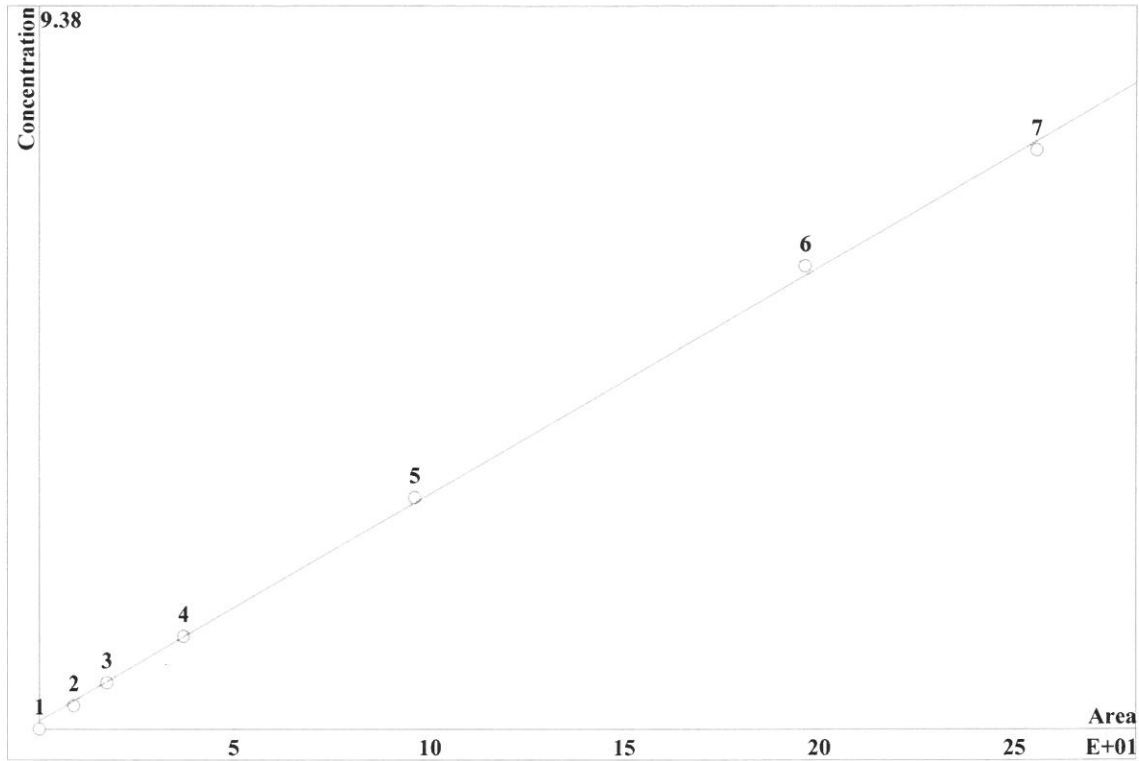


K3 = 0 K2 = 0 K1 = 0.587678 K0 = 2.15085
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.5279	8.733	0.3	20	11.45	Yes	
3	1.015	17.24	0.6	20	11.45	Yes	
4	2.119	37.01	1.2	20	11.45	Yes	
5	5.09	96.15	3	20	11.45	Yes	
6	9.875	196.3	6	20	11.45	Yes	
7	12.41	255.6	7.5	20	11.45	Yes	

CALIBRATION OF COMPONENT BR-

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 2.89714 \cdot A + 6.828$
 RSD: 3.738 %
 Correlation coefficient: 0.999409

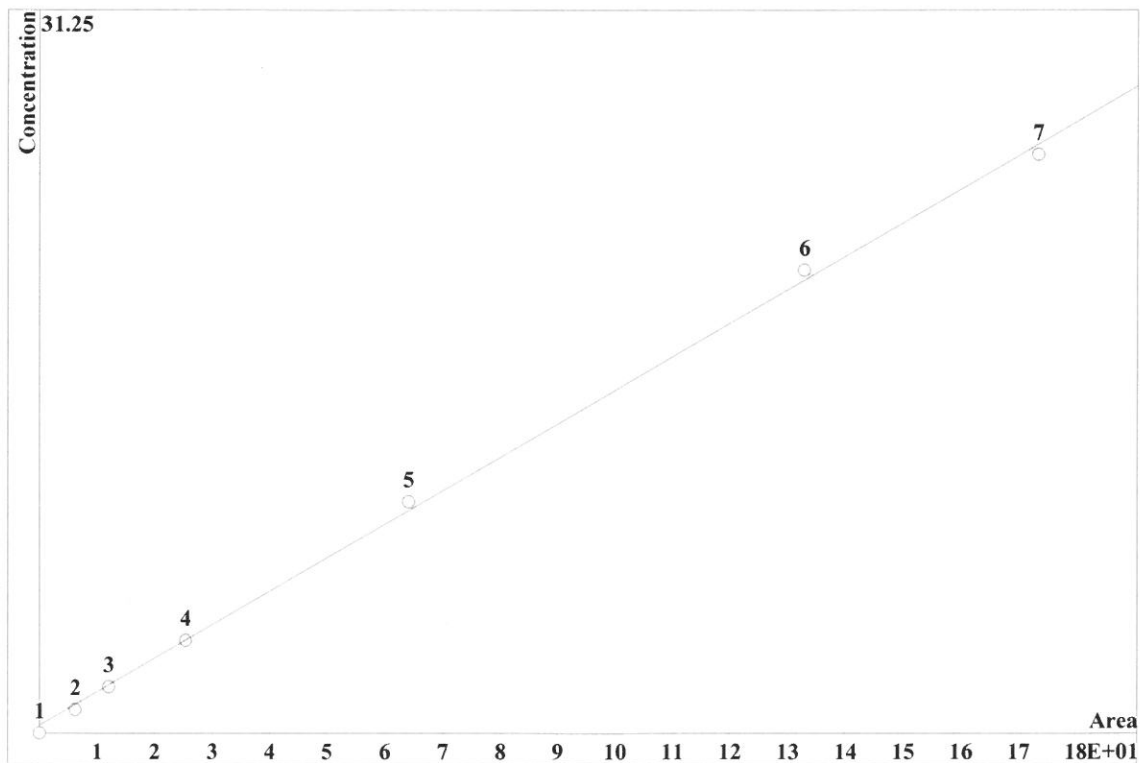

K3 = 0 K2 = 0 K1 = 2.89714 K0 = 6.828

Base: Area

Ref.channel: Cond

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.2998	6.248	1	20	15.03			Yes
3	0.5895	12.08	2	20	15.03			Yes
4	1.266	25.4	4	20	15.03			Yes
5	3.262	64.05	10	20	15.03			Yes
6	6.929	132.8	20	20	15.03			Yes
7	9.004	173.3	25	20	15.03			Yes

±□:□

CALIBRATION OF COMPONENT NO3

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 0.512801 \cdot A + 1.69346$
 RSD: 4.353 %
 Correlation coefficient: 0.999199

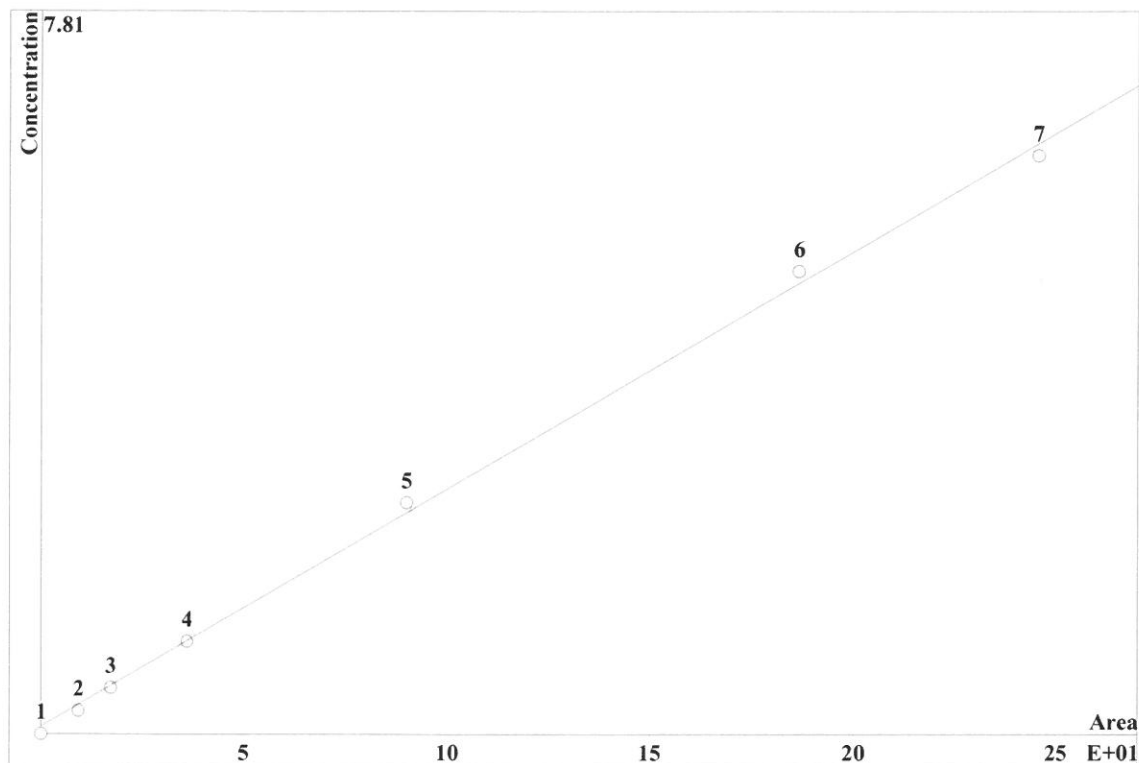

K3 = 0 K2 = 0 K1 = 0.512801 K0 = 1.69346

Base: Area

Ref.channel: Cond

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.3633	9.114	0.25	20	17.65		Yes
3	0.7016	17.18	0.5	20	17.65		Yes
4	1.484	36.12	1	20	17.65		Yes
5	3.76	90.04	2.5	20	17.65		Yes
6	7.858	186.7	5	20	17.65		Yes
7	10.16	245.6	6.25	20	17.65		Yes

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 1.04222 \cdot A - 1.17168$
 RSD: 3.359 %
 Correlation coefficient: 0.999523

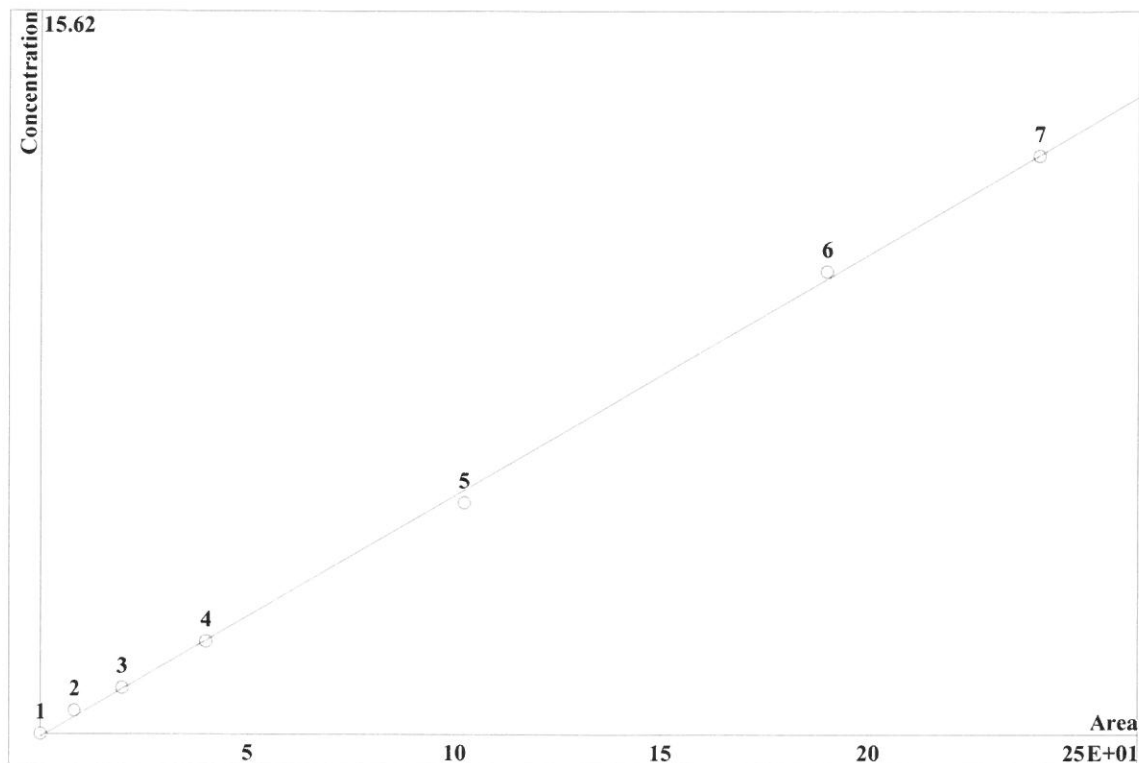

K3 = 0 K2 = 0 K1 = 1.04222 K0 = -1.17168

Base: Area

Ref.channel: Cond

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.1772	8.225	0.5	20	23.03		Yes
3	0.4669	19.91	1	20	23.03		Yes
4	0.8833	40.02	2	20	23.03		Yes
5	2.811	102.3	5	20	23.03		Yes
6	5.544	189.9	10	20	23.03		Yes
7	7.006	241.3	12.5	20	23.03		Yes

CALIBRATION OF COMPONENT SO4

Method: ANIONS 01-04-21.mtw
 Equation: $Q = 1.71085 \cdot A + 8.12037$
 RSD: 3.037 %
 Correlation coefficient: 0.999610

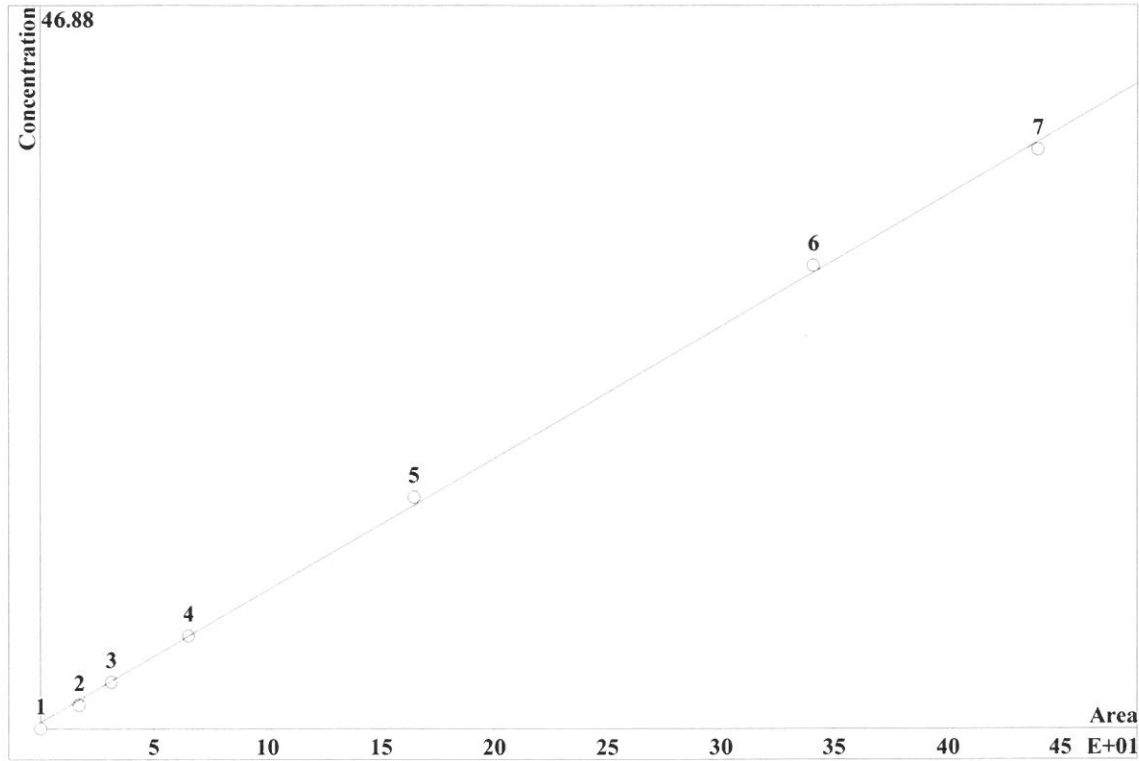

K3 = 0 K2 = 0 K1 = 1.71085 K0 = 8.12037
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0		0	0	0		0	No
2	0.483		17.03	1.5	20		26.99	Yes
3	0.9093		31.26	3	20		26.99	Yes
4	1.925		65.49	6	20		26.99	Yes
5	4.957		164.4	15	20		26.99	Yes
6	10.52		340.7	30	20		26.99	Yes
7	13.68		439.7	37.5	20		26.99	Yes

Report date: 1/5/2021 8:32:39 AM
Printed by: wet


Ident: STD1
Analysis from: 1/4/2021 6:42:29 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72890

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

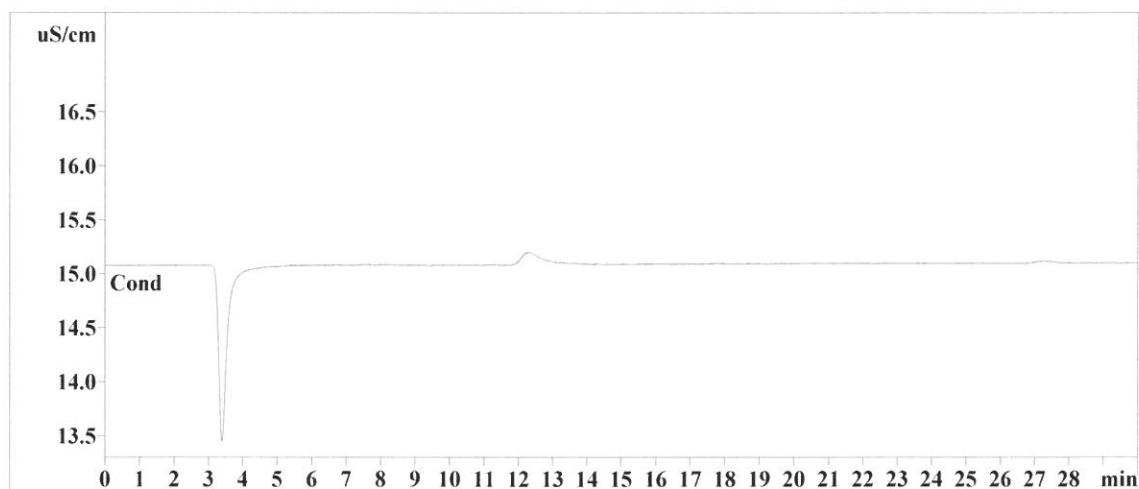

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:32:46 AM
Printed by: wet


Ident: STD2
Analysis from: 1/4/2021 7:15:23 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72891

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

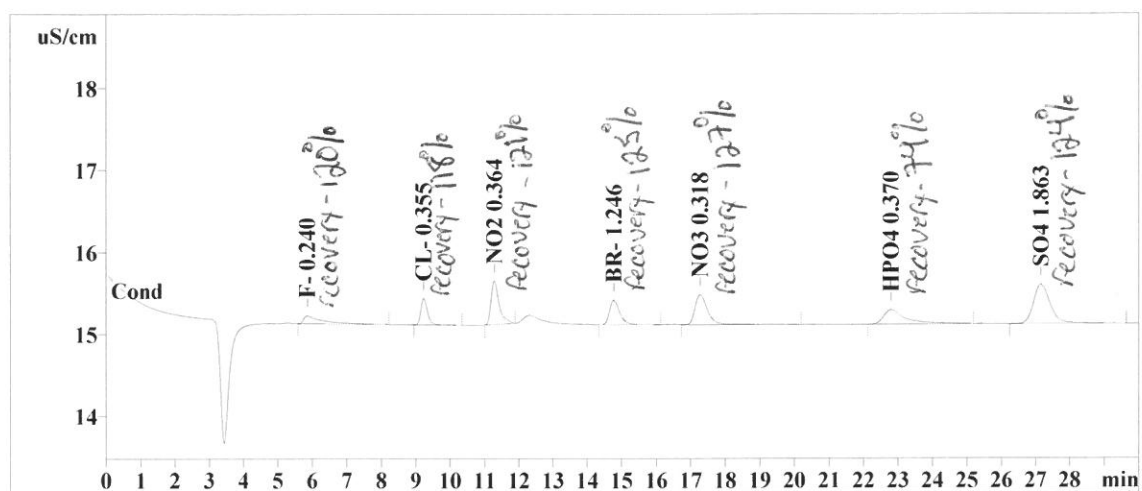

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.85	0.443	0.10	4.21	3.624	6.32	0.
2	9.22	0.197	0.32	14.20	4.331	7.56	0.
3	11.28	0.238	0.53	23.23	8.733	15.24	0.
4	14.77	0.309	0.30	13.17	6.248	10.90	0.
5	17.27	0.361	0.36	15.98	9.114	15.91	0.
6	22.79	0.574	0.18	7.78	8.225	14.35	0.
7	27.16	0.509	0.48	21.24	17.027	29.71	0.
7	30.00	0.376	2.27	99.82	57.303	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:32:54 AM
Printed by: wet


Ident: STD3
Analysis from: 1/4/2021 7:48:17 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72892

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

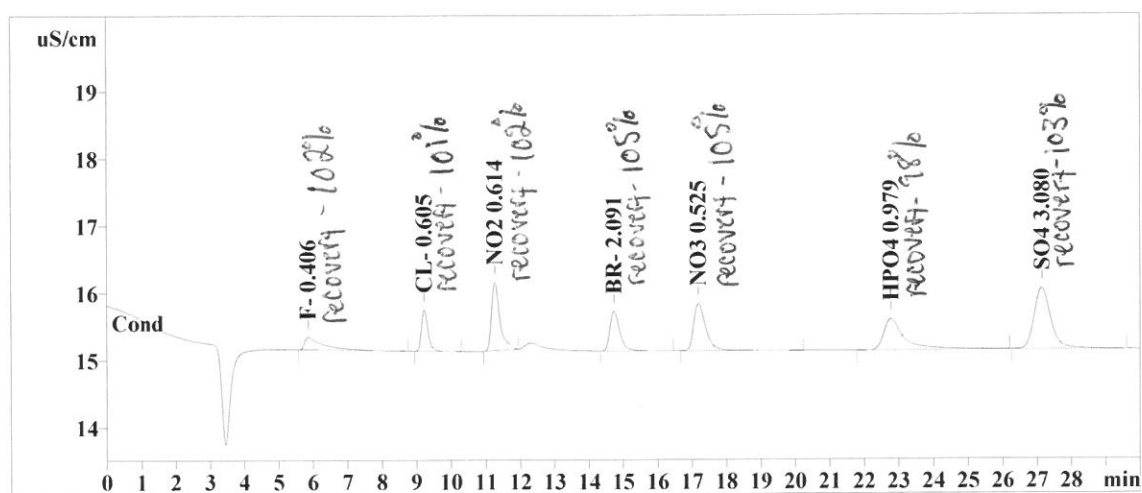

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.86	0.485	0.19	4.14	7.398	6.53	0.
2	9.22	0.197	0.61	13.64	8.137	7.19	0.
3	11.26	0.240	1.01	22.65	17.238	15.23	0.
4	14.72	0.303	0.59	13.15	12.081	10.67	0.
5	17.19	0.358	0.70	15.65	17.178	15.17	0.
6	22.78	0.524	0.47	10.40	19.907	17.59	0.
7	27.14	0.504	0.91	20.29	31.264	27.62	0.
7	30.00	0.373	4.48	99.92	113.203	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:33:01 AM
Printed by: wet


Ident: STD4
Analysis from: 1/4/2021 8:21:11 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72893

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

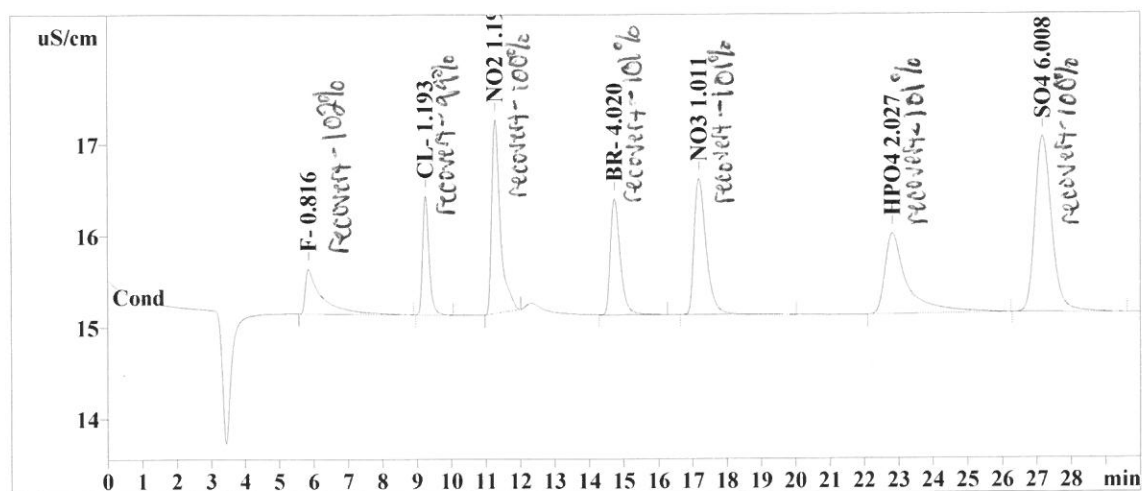

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.85	0.377	0.49	5.16	16.712	7.03	0.
2	9.24	0.195	1.30	13.71	17.094	7.19	0.
3	11.27	0.244	2.12	22.39	37.005	15.56	0.
4	14.72	0.298	1.27	13.37	25.395	10.68	0.
5	17.18	0.359	1.48	15.68	36.124	15.19	0.
6	22.82	0.545	0.88	9.33	40.016	16.82	0.
7	27.17	0.505	1.93	20.34	65.490	27.54	0.
7	30.00	0.361	9.46	99.98	237.836	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:33:07 AM
Printed by: wet


Ident: STD5
Analysis from: 1/4/2021 8:54:04 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72894

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

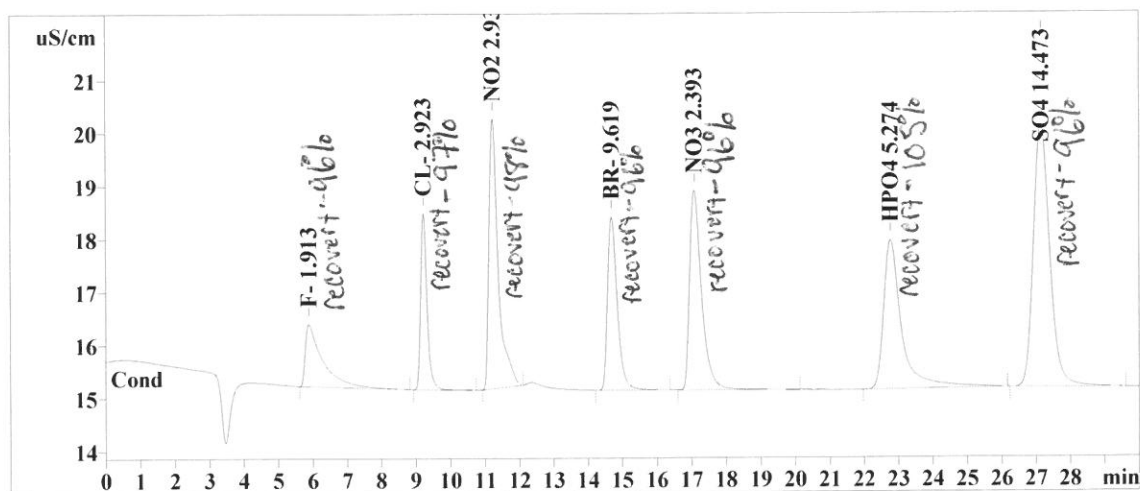

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.448	1.17	4.81	41.636	6.91	0.
2	9.21	0.192	3.32	13.61	43.468	7.22	0.
3	11.21	0.260	5.09	20.88	96.149	15.97	0.
4	14.68	0.292	3.26	13.38	64.045	10.64	0.
5	17.08	0.351	3.76	15.42	90.039	14.95	0.
6	22.77	0.478	2.81	11.53	102.333	17.00	0.
7	27.14	0.497	4.96	20.34	164.446	27.31	0.
7	30.00	0.360	24.37	99.99	602.117	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:33:13 AM
Printed by: wet


Ident: STD6
Analysis from: 1/4/2021 9:26:58 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72895

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

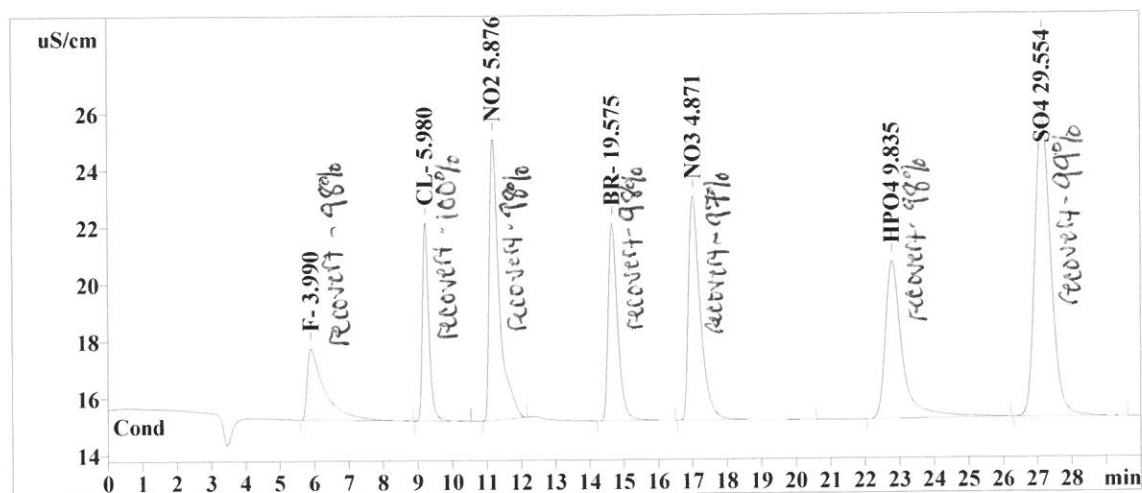

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.91	0.448	2.51	4.99	88.835	7.25	0.
2	9.22	0.191	6.96	13.86	90.070	7.35	0.
3	11.18	0.271	9.88	19.68	196.312	16.02	0.
4	14.66	0.285	6.93	13.81	132.775	10.84	0.
5	17.02	0.347	7.86	15.66	186.682	15.24	0.
6	22.79	0.461	5.54	11.05	189.862	15.50	0.
7	27.15	0.489	10.51	20.95	340.742	27.81	0.
7	30.00	0.356	50.18	100.00	1225.278	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:33:19 AM
Printed by: wet


Ident: STD7
Analysis from: 1/4/2021 9:59:52 PM
File: _2021-01-04_

Last save: 1/5/2021 8:29:36 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72896

Last save: 1/4/2021 9:56:46 PM

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

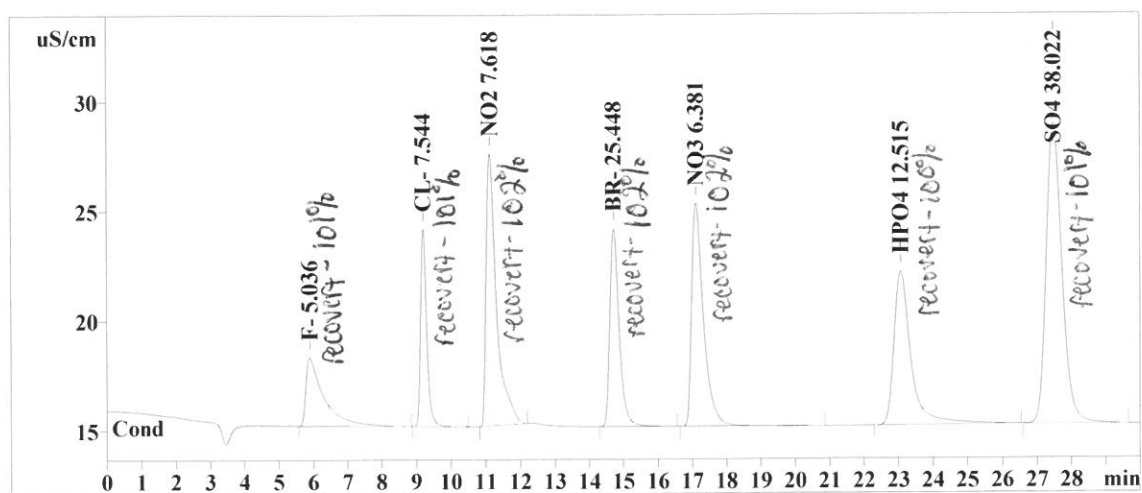

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.90	0.457	3.11	4.83	112.605	7.12	0.
2	9.20	0.187	8.99	13.97	113.910	7.20	0.
3	11.12	0.281	12.40	19.28	255.603	16.16	0.
4	14.71	0.286	9.00	13.99	173.323	10.96	0.
5	17.11	0.352	10.15	15.78	245.571	15.52	0.
6	23.07	0.468	7.01	10.89	241.285	15.25	0.
7	27.48	0.487	13.68	21.26	439.730	27.80	0.
7	30.00	0.360	64.35	99.99	1582.026	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:33:30 AM
Printed by: wet


Ident: ICV
Analysis from: 1/4/2021 10:32:46 PM
File: _2021-01-04_

Last save: 1/4/2021 11:02:34 PM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72897

Last save: 1/4/2021 10:29:40 PM

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

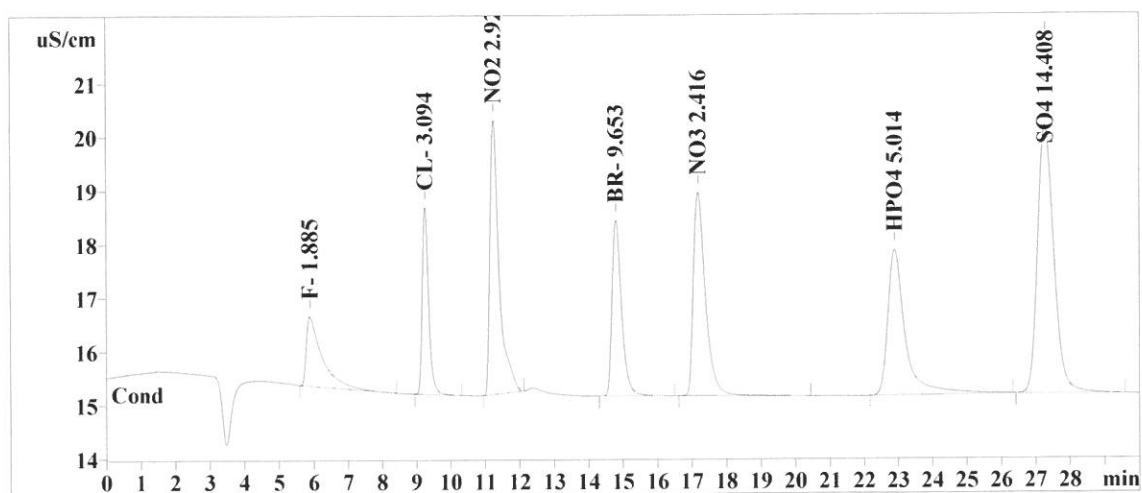

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.413	1.29	5.24	41.009	6.85	0.
2	9.25	0.196	3.48	14.12	46.081	7.69	0.
3	11.24	0.257	5.11	20.71	95.727	15.98	0.
4	14.79	0.293	3.27	13.28	64.282	10.73	0.
5	17.18	0.352	3.79	15.37	90.937	15.18	0.
6	22.89	0.476	2.72	11.02	97.346	16.25	0.
7	27.27	0.493	5.00	20.26	163.690	27.32	0.
7	30.00	0.354	24.66	99.99	599.072	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/5/2021 8:33:37 AM
Printed by: wet


Ident: ICB
Analysis from: 1/4/2021 11:05:40 PM
File: _2021-01-04_

Last save: 1/4/2021 11:35:28 PM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72898

Last save: 1/4/2021 10:29:40 PM

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

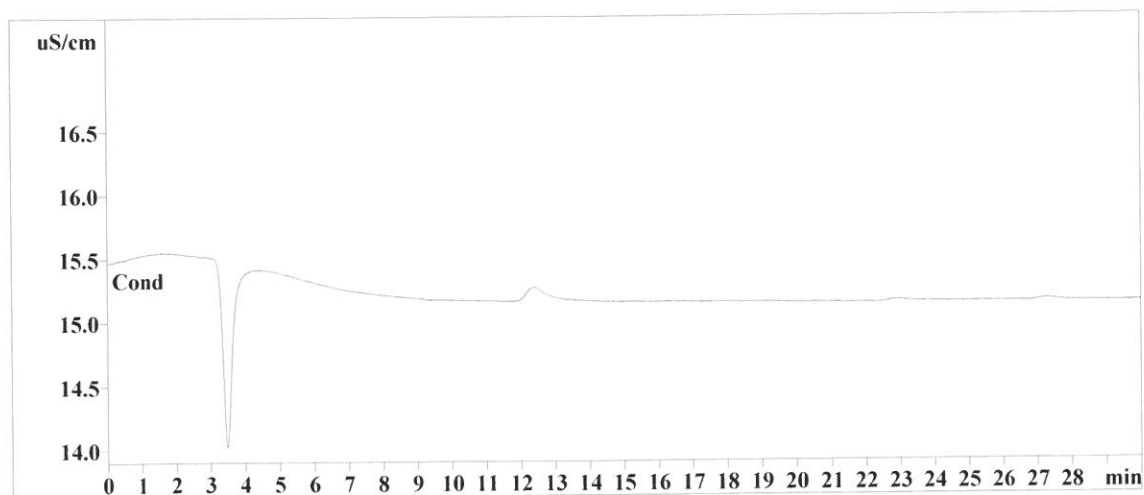

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:38:12 AM
Printed by: wet


Ident: CCV
Analysis from: 1/8/2021 10:14:31 AM
File: _2021-01-08_

Last save: 1/8/2021 10:43:50 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72960

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

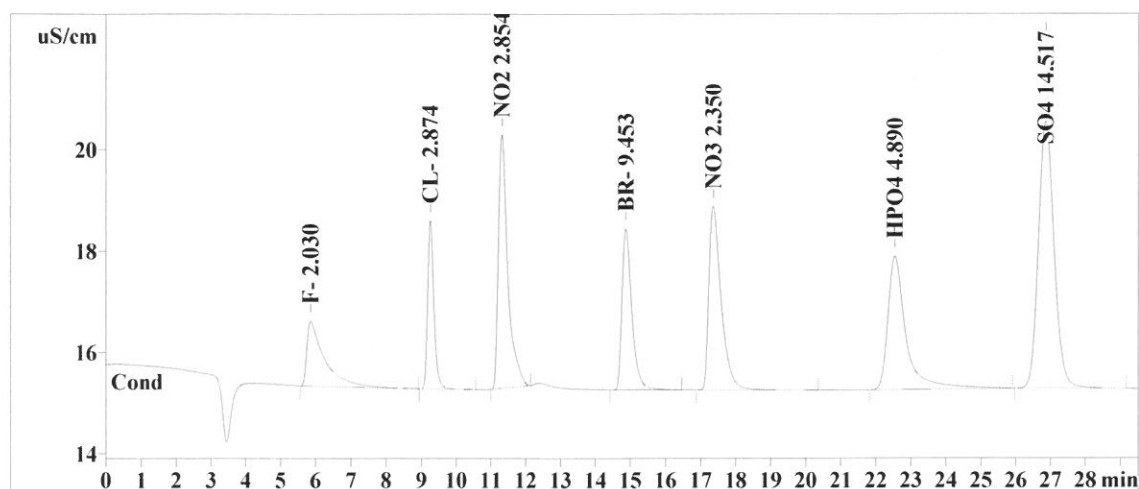

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.87	0.441	1.28	5.25	44.312	7.49	0.
2	9.25	0.191	3.31	13.64	42.726	7.22	0.
3	11.31	0.261	5.00	20.59	93.468	15.80	0.
4	14.87	0.293	3.18	13.07	62.899	10.63	0.
5	17.35	0.358	3.62	14.91	88.336	14.93	0.
6	22.53	0.472	2.63	10.85	94.954	16.05	0.
7	26.85	0.474	5.27	21.68	164.960	27.88	0.
7	29.50	0.356	24.29	100.00	591.655	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:38:19 AM
Printed by: wet


Ident: CCB
Analysis from: 1/8/2021 10:48:30 AM
File: _2021-01-08_

Last save: 1/8/2021 11:17:48 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72961

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

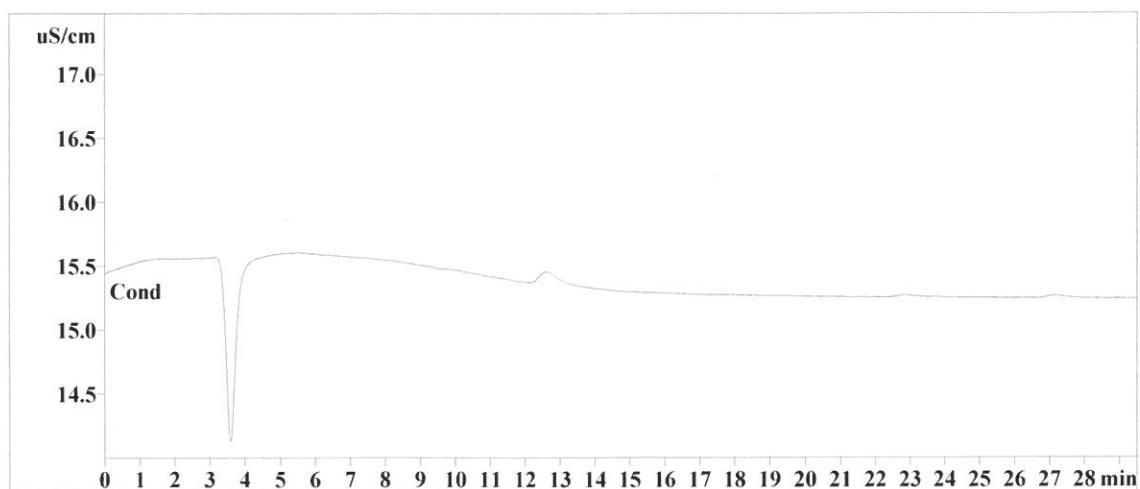

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:38:25 AM
Printed by: wet


Ident: LB112696BLW
Analysis from: 1/8/2021 11:20:54 AM
File: _2021-01-08_

Last save: 1/11/2021 10:38:04 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72962

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

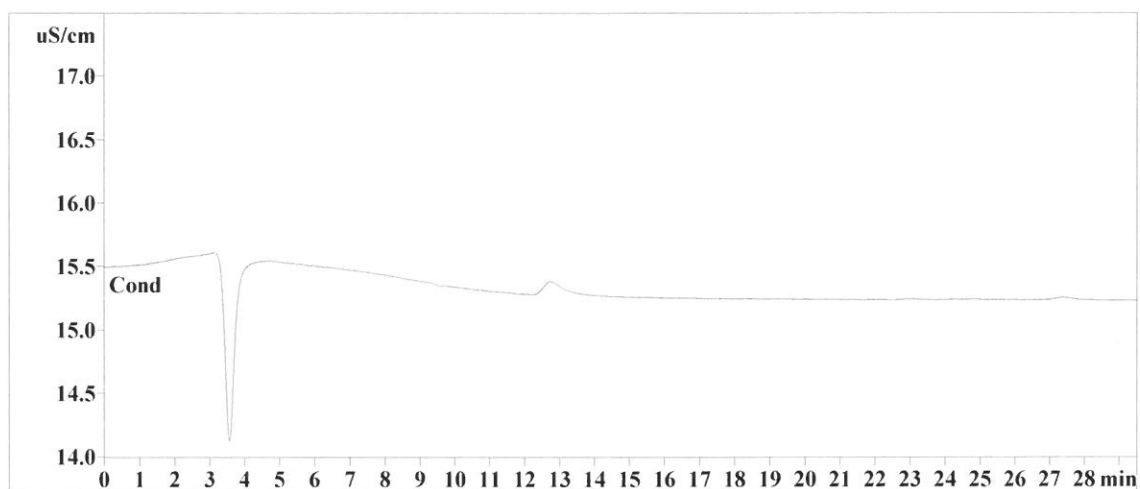

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:38:31 AM
Printed by: wet


Ident: LB112696BSW
Analysis from: 1/8/2021 11:53:18 AM
File: _2021-01-08_

Last save: 1/11/2021 10:38:04 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72963

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

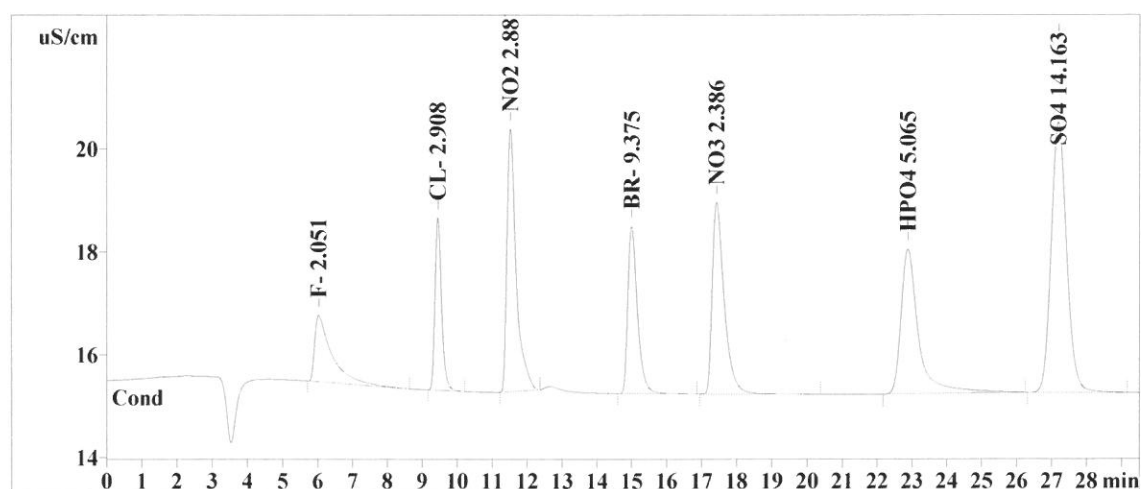

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	6.02	0.452	1.29	5.21	44.779	7.54	0.
2	9.44	0.192	3.35	13.54	43.246	7.28	0.
3	11.51	0.259	5.10	20.60	94.403	15.90	0.
4	15.00	0.285	3.25	13.10	62.361	10.50	0.
5	17.42	0.355	3.72	15.02	89.739	15.12	0.
6	22.87	0.460	2.81	11.34	98.313	16.56	0.
7	27.18	0.464	5.25	21.18	160.815	27.09	0.
7	29.50	0.352	24.76	99.99	593.656	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:39:18 AM
Printed by: wet


Ident: M1046-01
Analysis from: 1/8/2021 12:39:27 PM
File: _2021-01-08_

Last save: 1/11/2021 10:39:16 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72964

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

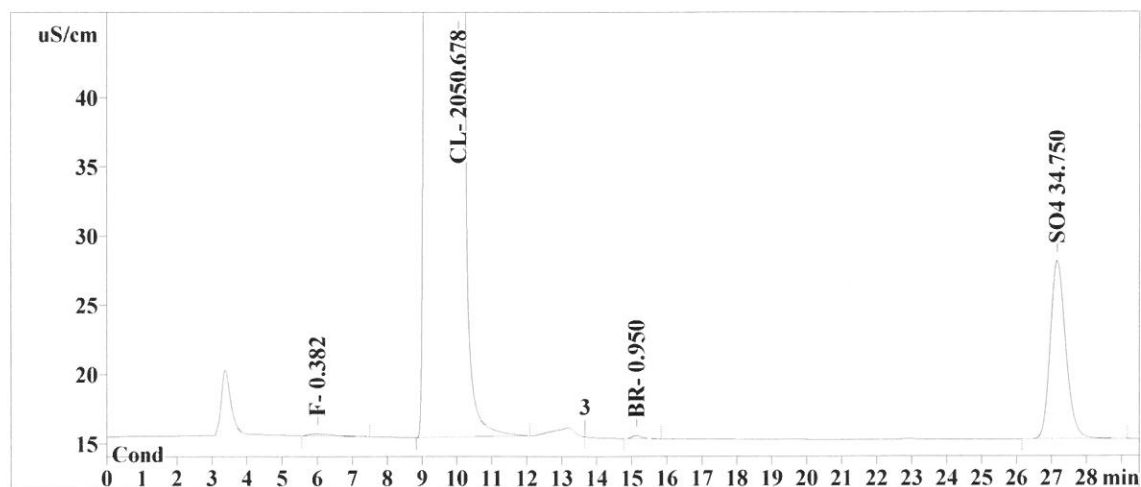

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	6.01	0.728	0.14	0.02	6.864	0.02	0.
2	10.03	0.777	712.53	98.14	31258.796	98.70	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	15.13	0.287	0.22	0.03	4.204	0.01	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	27.16	0.471	12.86	1.77	401.481	1.27	0.
7	29.50	0.323	725.75	99.96	31671.344	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:39:34 AM
Printed by: wet


Ident: M1046-01DUP
Analysis from: 1/8/2021 1:11:51 PM
File: _2021-01-08_

Last save: 1/11/2021 10:38:04 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72965

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

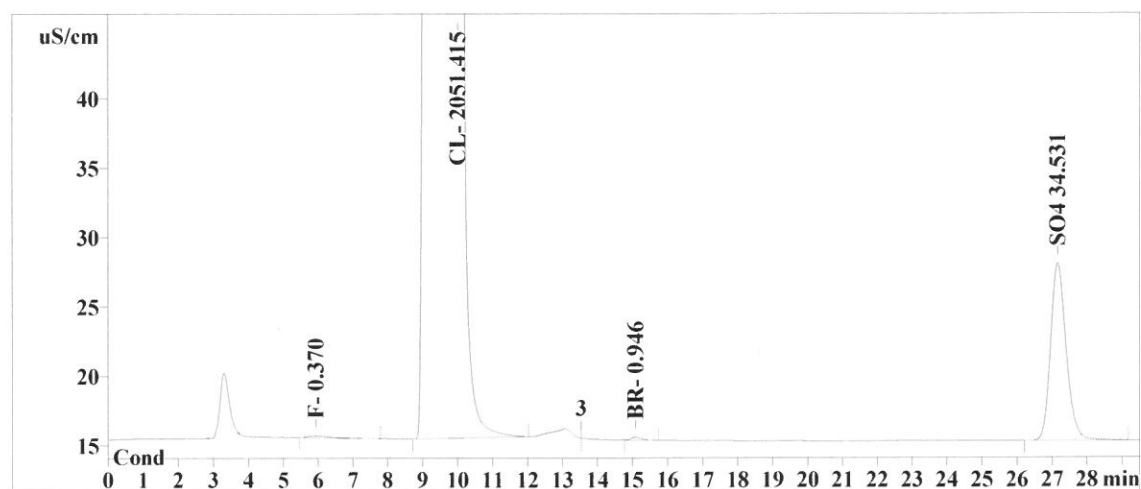

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.93	0.699	0.14	0.02	6.575	0.02	0.
2	9.99	0.777	711.49	98.15	31270.031	98.71	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	15.09	0.290	0.22	0.03	4.173	0.01	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	27.15	0.471	12.79	1.76	398.924	1.26	0.
7	29.50	0.320	724.63	99.96	31679.703	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:40:00 AM
Printed by: wet


Ident: M1046-01MS
Analysis from: 1/8/2021 1:44:15 PM
File: _2021-01-08_

Last save: 1/11/2021 10:40:00 AM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72966

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

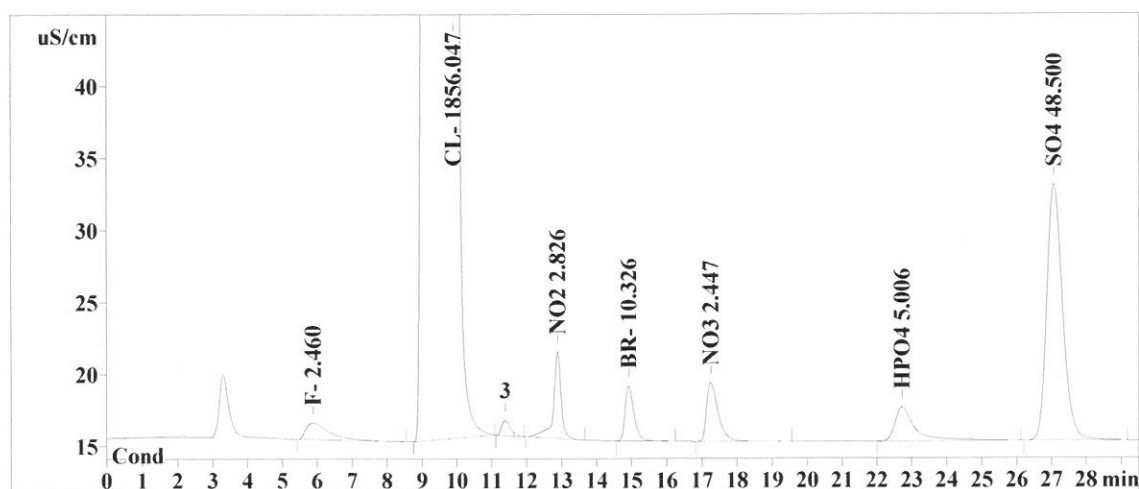

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.670	1.16	0.16	54.071	0.18	0.
2	9.89	0.730	685.22	94.94	28291.896	96.63	0.
3	12.89	0.194	6.02	0.83	92.513	0.32	0.
4	14.92	0.273	3.81	0.53	68.928	0.24	0.
5	17.25	0.337	4.07	0.56	92.148	0.31	0.
6	22.72	0.507	2.39	0.33	97.185	0.33	0.
7	27.06	0.479	17.78	2.46	562.218	1.92	0.
7	29.50	0.456	720.45	99.82	29258.958	99.94	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:40:15 AM
 Printed by: wet


Ident: M1046-01MSD
 Analysis from: 1/8/2021 2:49:03 PM
 File: _2021-01-08_

Last save: 1/11/2021 10:40:16 AM

Method: ANIONS 01-04-21.mtw
 Run operator: wet
 Analysis number: 72968

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
 : AM/AP
 Vial number: 11
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

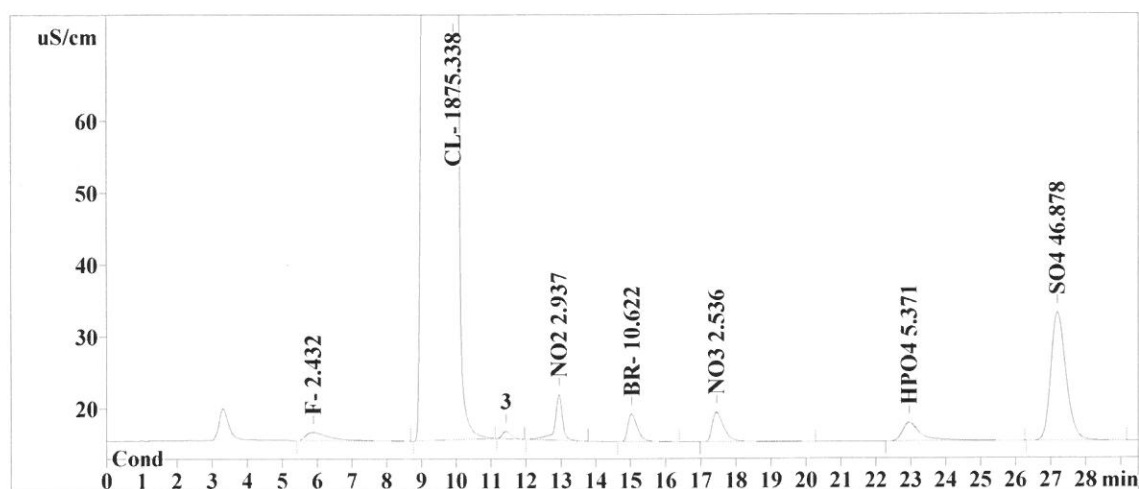

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.649	1.12	0.16	53.440	0.18	0.
2	9.91	0.739	685.35	94.85	28585.971	96.68	0.
3	12.94	0.195	6.29	0.87	96.286	0.33	0.
4	15.04	0.279	3.84	0.53	70.973	0.24	0.
5	17.44	0.347	4.10	0.57	95.624	0.32	0.
6	22.95	0.490	2.64	0.36	104.187	0.35	0.
7	27.19	0.461	17.82	2.47	543.262	1.84	0.
7	29.50	0.451	721.16	99.80	29549.743	99.94	0.

This report has been created by IC Net
 METROHM LTD

Report date: 1/11/2021 10:40:37 AM
Printed by: wet


Ident: M1046-01DLX500
Analysis from: 1/8/2021 3:21:27 PM
File: _2021-01-08_

Last save: 1/8/2021 4:07:54 PM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72969

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

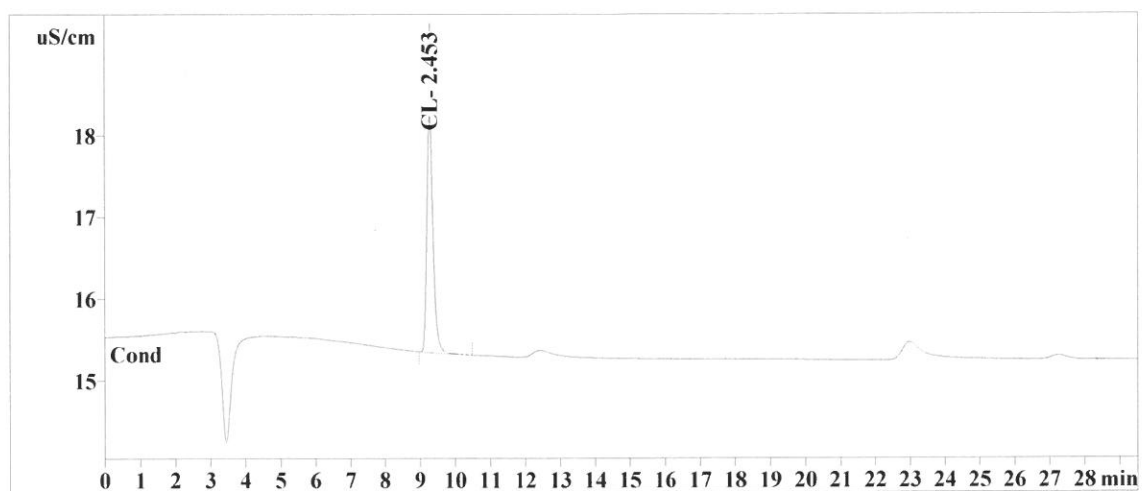

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	9.27	0.187	2.89	100.01	36.312	100.00	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	0.00	0.000	0.00	0.00	0.000	0.00	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	29.50	0.027	2.89	100.01	36.312	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:41:08 AM
Printed by: wet


Ident: L1062-03
Analysis from: 1/8/2021 4:32:57 PM
File: _2021-01-08_

Last save: 1/8/2021 5:19:00 PM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72971

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

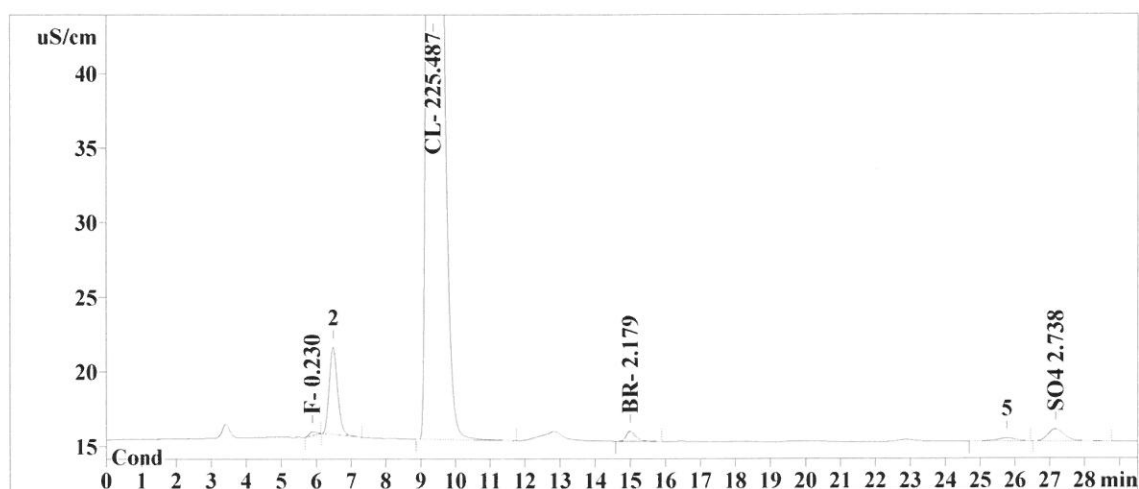

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.223	0.25	0.14	3.396	0.09	0.
2	9.35	0.297	168.25	95.57	3436.158	95.83	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	15.00	0.287	0.66	0.38	12.687	0.35	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	27.16	0.498	0.82	0.46	27.261	0.76	0.
7	29.50	0.186	169.98	96.55	3479.502	97.04	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:41:26 AM
Printed by: wet


Ident: CCV
Analysis from: 1/8/2021 5:38:32 PM
File: _2021-01-08_

Last save: 1/8/2021 6:07:50 PM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72973

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

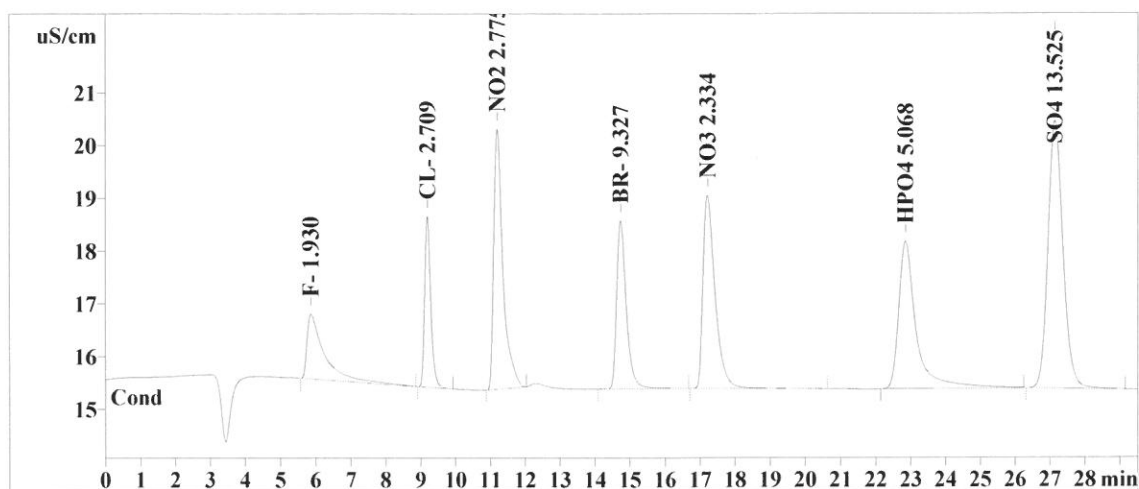

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.87	0.421	1.23	5.08	42.032	7.32	0.
2	9.18	0.186	3.23	13.42	40.214	7.00	0.
3	11.18	0.258	4.93	20.45	90.769	15.80	0.
4	14.72	0.287	3.18	13.21	62.029	10.80	0.
5	17.20	0.351	3.66	15.18	87.734	15.27	0.
6	22.84	0.459	2.79	11.59	98.386	17.12	0.
7	27.13	0.458	5.07	21.05	153.366	26.69	0.
7	29.50	0.346	24.10	99.99	574.531	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/11/2021 10:41:38 AM
Printed by: wet


Ident: CCB
Analysis from: 1/8/2021 6:10:56 PM
File: _2021-01-08_

Last save: 1/8/2021 6:40:14 PM

Method: ANIONS 01-04-21.mtw
Run operator: wet
Analysis number: 72974

Last save: 1/6/2021 10:42:44 AM

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

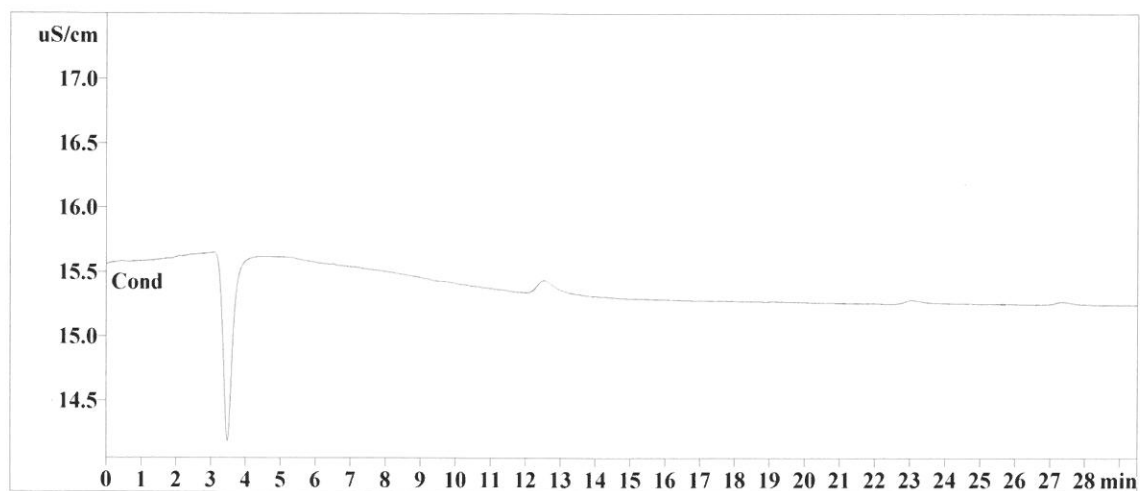

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD