


LB112744

7471B

INSTRUMENT ID: CV1

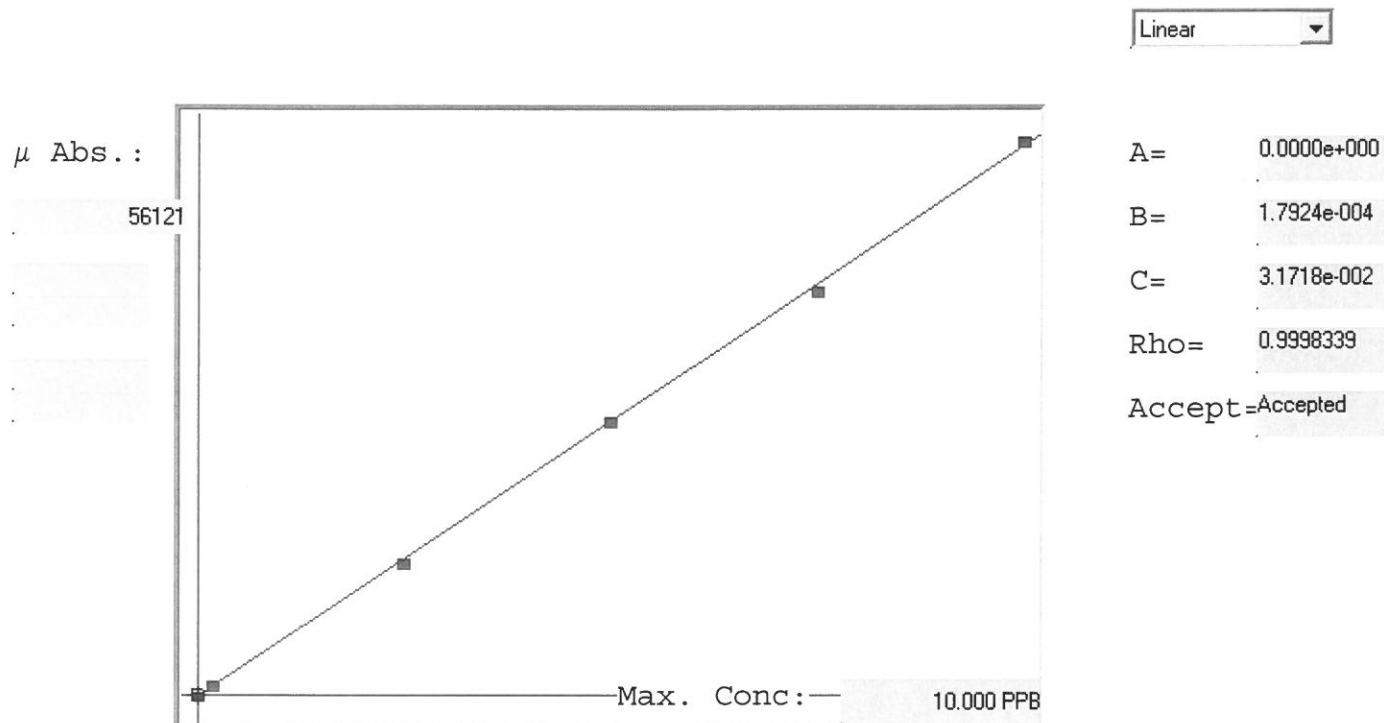

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.044	0.044	66	0.000	66				
0.2	0.200	0.222	0.022	1060	0.0 %	1060				
2.5	2.500	2.448	-0.052	13479	0.0 %	13479				
5.0	5.000	5.012	0.012	27787	0.0 %	27787				
7.5	7.500	7.383	-0.117	41015	0.0 %	41015				
10.0	10.000	10.091	0.091	56121	0.0 %	56121				

LB112724 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 11 Jan 2021 16:06:21

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	66	-	0.0000	7471B	PPB	11 Jan 2021 16:07:21	S	Std
0.2 - 1	50.2	1060	-	0.2000	7471B	PPB	11 Jan 2021 16:09:38	S	Std
2.5 - 1	52.5	13479	-	2.5000	7471B	PPB	11 Jan 2021 16:11:55	S	Std
5.0 - 1	55	27787	-	5.0000	7471B	PPB	11 Jan 2021 16:14:12	S	Std
7.5 - 1	57.5	41015	-	7.5000	7471B	PPB	11 Jan 2021 16:16:29	S	Std
10.0 - 1	58	56121	-	10.0000	7471B	PPB	11 Jan 2021 16:18:45	S	Std
ICV67 - 1	ICV67	20682	3.7389	-	7471B	PPB	11 Jan 2021 16:21:44	U	SMPL
ICB67 - 1	ICB67	-48	0.0231	-	7471B	PPB	11 Jan 2021 16:23:59	U	SMPL
CCV04 - 1	CCV04	27694	4.9957	-	7471B	PPB	11 Jan 2021 16:26:14	U	SMPL
CCB04 - 1	CCB04	-58	0.0213	-	7471B	PPB	11 Jan 2021 16:28:29	U	SMPL
CRA - 1	CRA	1030	0.2163	-	7471B	PPB	11 Jan 2021 16:30:44	U	SMPL
HighStd - 1	HighStd	55439	9.9689	-	7471B	PPB	11 Jan 2021 16:32:59	U	SMPL
ChkStd - 1	ChkStd	38379	6.9110	-	7471B	PPB	11 Jan 2021 16:37:49	U	SMPL
PB134034BL - 1	PBS	-57	0.0215	-	7471B	PPB	11 Jan 2021 16:40:05	U	SMPL
PB134034BS - 1	LCSS	18958	3.4298	-	7471B	PPB	11 Jan 2021 16:42:21	U	SMPL
M1055-01 - 1	SA-01-010821	662	0.1504	-	7471B	PPB	11 Jan 2021 16:44:37	U	SMPL
M1055-01DUP - 1	SA-01-010821DUP	764	0.1687	-	7471B	PPB	11 Jan 2021 16:49:36	U	SMPL
M1055-01MS - 1	SA-01-010821MS	19277	3.4870	-	7471B	PPB	11 Jan 2021 16:51:52	U	SMPL
M1055-01MSD - 1	SA-01-010821MSD	18939	3.4264	-	7471B	PPB	11 Jan 2021 16:54:09	U	SMPL
M1056-01 - 1	CL-01-010821	2383	0.4589	-	7471B	PPB	11 Jan 2021 16:56:25	U	SMPL
CCV05 - 1	CCV05	26664	4.8111	-	7471B	PPB	11 Jan 2021 16:58:40	U	SMPL
CCB05 - 1	CCB05	-49	0.0229	-	7471B	PPB	11 Jan 2021 17:00:56	U	SMPL
M1059-01 - 1	TR-04-010821	1095	0.2280	-	7471B	PPB	11 Jan 2021 17:03:11	U	SMPL
M1061-01 - 1	245657	469	0.1158	-	7471B	PPB	11 Jan 2021 17:05:27	U	SMPL
M1062-01 - 1	HD-FDC	8560	1.5661	-	7471B	PPB	11 Jan 2021 17:07:42	U	SMPL
M1068-01 - 1	FK-GF-02-066-A	7950	1.4567	-	7471B	PPB	11 Jan 2021 17:09:58	U	SMPL
M1068-03 - 1	FK-GF-02-066-B	8501	1.5555	-	7471B	PPB	11 Jan 2021 17:12:14	U	SMPL
M1069-01 - 1	FK-GF-02-065-A	6685	1.2300	-	7471B	PPB	11 Jan 2021 17:14:31	U	SMPL
M1069-03 - 1	FK-GF-02-065-B	6918	1.2717	-	7471B	PPB	11 Jan 2021 17:16:48	U	SMPL
M1055-01LX5 - 1		130	0.0550	-	7471B	PPB	11 Jan 2021 17:19:05	U	SMPL
M1055-01A - 1		20811	3.7620	-	7471B	PPB	11 Jan 2021 17:21:21	U	SMPL
CCV06 - 1	CCV06	26628	4.8047	-	7471B	PPB	11 Jan 2021 17:23:37	U	SMPL
CCB06 - 1	CCB06	-49	0.0229	-	7471B	PPB	11 Jan 2021 17:25:53	U	SMPL