


LB112757

7471B

INSTRUMENT ID: CV1

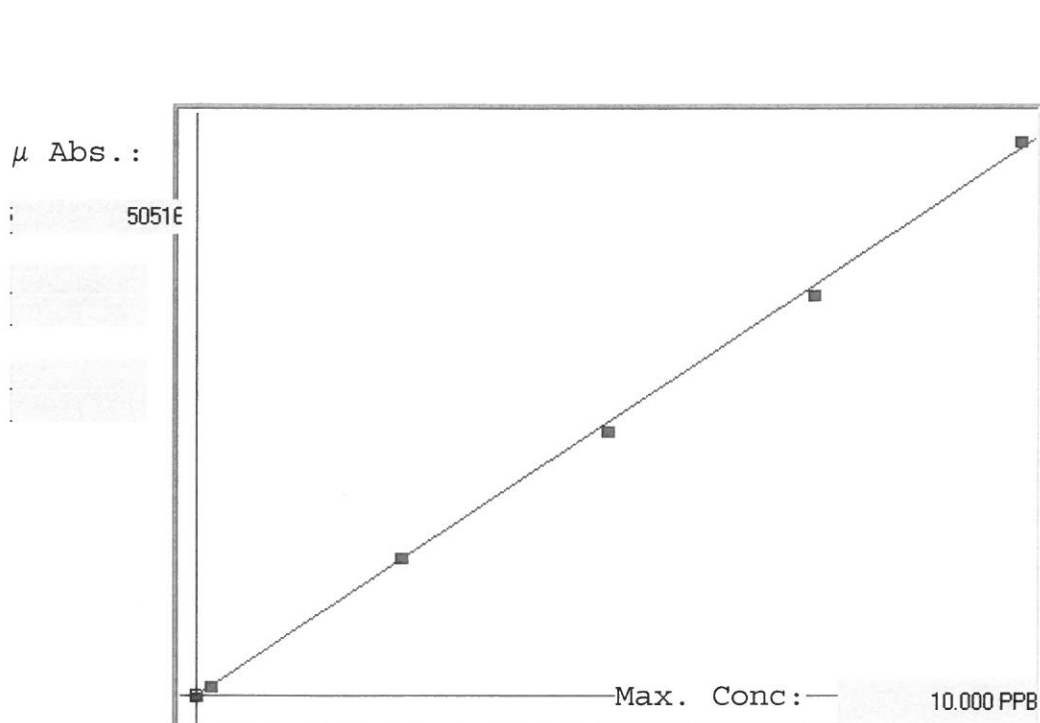

Linear

A= 0.0000e+000

B= 2.0031e-004

C= 2.2177e-002

Rho= 0.9996515

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/o D
0.0	0.000	0.041	0.041	92	0.000	92					-
0.2	0.200	0.222	0.022	996	0.0 %	996					11
2.5	2.500	2.551	0.051	12624	0.0 %	12624					2
5.0	5.000	4.877	-0.123	24236	0.0 %	24236					-2
7.5	7.500	7.369	-0.131	36677	0.0 %	36677					-2
10.0	10.000	10.141	0.141	50516	0.0 %	50516					1

LB112757 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 13 Jan 2021 11:30:32

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	92	-	0.0000	7471B	PPB	13 Jan 2021 11:32:04	S	Std
0.2 - 1	50.2	996	-	0.2000	7471B	PPB	13 Jan 2021 11:34:21	S	Std
2.5 - 1	52.5	12624	-	2.5000	7471B	PPB	13 Jan 2021 11:36:39	S	Std
5.0 - 1	55	24236	-	5.0000	7471B	PPB	13 Jan 2021 11:38:56	S	Std
7.5 - 1	57.1	36677	-	7.5000	7471B	PPB	13 Jan 2021 11:41:13	S	Std
10.0 - 1	511	50516	-	10.0000	7471B	PPB	13 Jan 2021 11:43:29	S	Std
ICV69 - 1	ICV69	19198	3.8677	-	7471B	PPB	13 Jan 2021 11:46:12	U	SMPL
ICB69 - 1	ICB69	111	0.0444	-	7471B	PPB	13 Jan 2021 11:48:27	U	SMPL
CCV17 - 1	CCV17	24144	4.8585	-	7471B	PPB	13 Jan 2021 11:50:42	U	SMPL
CCB17 - 1	CCB17	76	0.0374	-	7471B	PPB	13 Jan 2021 11:52:57	U	SMPL
CRA - 1	CRA	951	0.2127	-	7471B	PPB	13 Jan 2021 11:55:12	U	SMPL
HighStd - 1	HighStd	49395	9.9165	-	7471B	PPB	13 Jan 2021 11:57:27	U	SMPL
ChkStd - 1	ChkStd	33659	6.7644	-	7471B	PPB	13 Jan 2021 11:59:42	U	SMPL
PB134083BL - 1	PBS	-44	0.0134	-	7471B	PPB	13 Jan 2021 12:01:59	U	SMPL
PB134083BS - 1	LCSS	16927	3.4128	-	7471B	PPB	13 Jan 2021 12:04:16	U	SMPL
M1073-01 - 1	VNJ-217	767	0.1758	-	7471B	PPB	13 Jan 2021 12:06:33	U	SMPL
M1075-01 - 1	72-11977	2080	0.4388	-	7471B	PPB	13 Jan 2021 12:08:50	U	SMPL
M1075-03 - 1	7	926	0.2077	-	7471B	PPB	13 Jan 2021 12:11:07	U	SMPL
M1076-01 - 1	OR-03-011121	8014	1.6275	-	7471B	PPB	13 Jan 2021 12:13:25	U	SMPL
M1076-01DUP - 1	OR-03-011121DUP	8040	1.6327	-	7471B	PPB	13 Jan 2021 12:18:23	U	SMPL
CCV18 - 1	CCV18	26718	5.3740	-	7471B	PPB	13 Jan 2021 12:21:33	U	SMPL
CCB18 - 1	CCB18	123	0.0468	-	7471B	PPB	13 Jan 2021 12:23:48	U	SMPL
M1076-01MS - 1	OR-03-011121MS	30347	6.1010	-	7471B	PPB	13 Jan 2021 12:26:03	U	SMPL
M1076-01MSD - 1	OR-03-011121MSD	28713	5.7737	-	7471B	PPB	13 Jan 2021 12:28:19	U	SMPL
M1077-01 - 1	JC-03-011121-A	3453	0.7138	-	7471B	PPB	13 Jan 2021 12:30:34	U	SMPL
M1077-03 - 1	JC-03-011121-B	3642	0.7517	-	7471B	PPB	13 Jan 2021 12:32:50	U	SMPL
M1078-01 - 1	NB-07-011121	1577	0.3381	-	7471B	PPB	13 Jan 2021 12:35:07	U	SMPL
M1076-01LX5 - 1		1969	0.4166	-	7471B	PPB	13 Jan 2021 12:37:23	U	SMPL
M1076-01A - 1		28742	5.7795	-	7471B	PPB	13 Jan 2021 12:39:40	U	SMPL
CCV19 - 1	CCV19	26103	5.2509	-	7471B	PPB	13 Jan 2021 12:41:57	U	SMPL
CCB19 - 1	CCB19	109	0.0440	-	7471B	PPB	13 Jan 2021 12:44:14	U	SMPL