


LB112863

7471B

INSTRUMENT ID: QV2

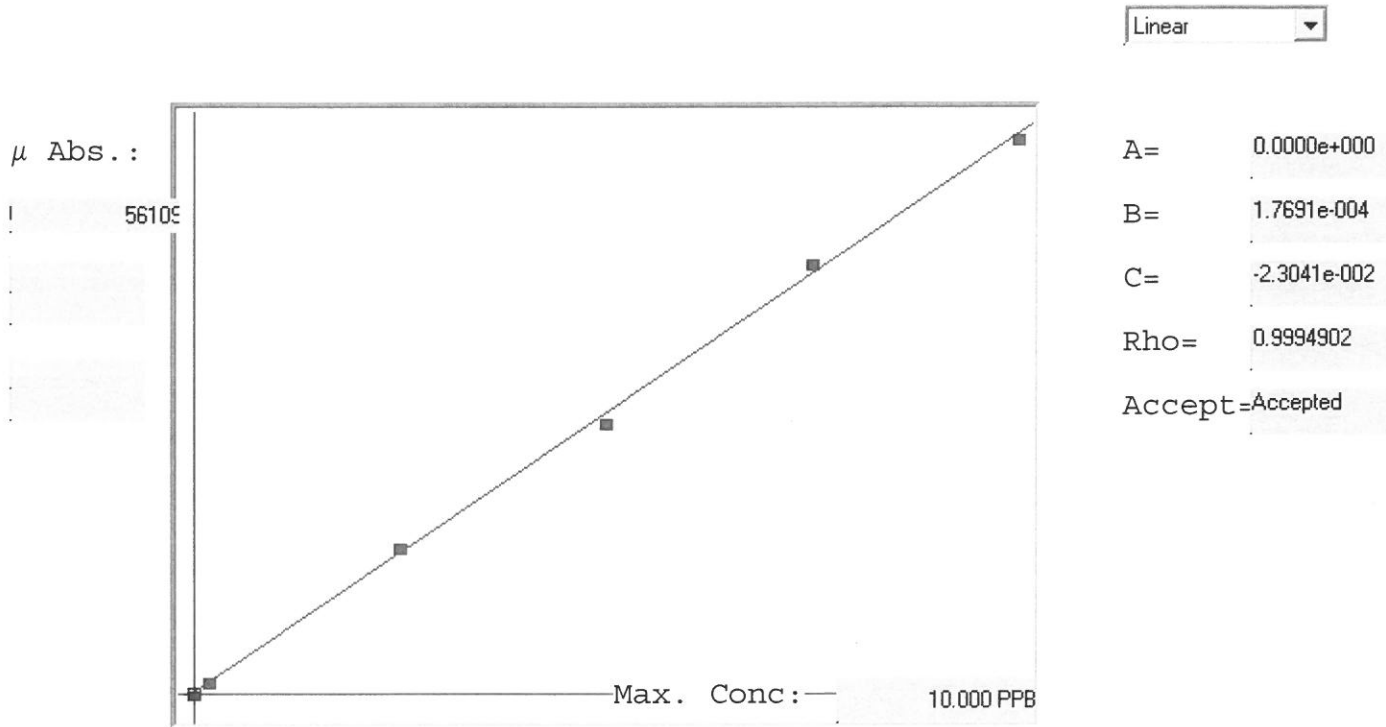

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.012	-0.012	65	0.000	65					
0.2	0.200	0.185	-0.015	1176	0.0 %	1176					-8
2.5	2.500	2.589	0.089	14765	0.0 %	14765					4
5.0	5.000	4.837	-0.163	27471	0.0 %	27471					-3
7.5	7.500	7.697	0.197	43641	0.0 %	43641					3
10.0	10.000	9.903	-0.097	56109	0.0 %	56109					-1

LB112863 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 20 Jan 2021 15:28:03				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	65	-	0.00007471B	PPB	20 Jan 2021 15:29:05	S	Std
0.2 - 1	50.2	1176	-	0.20007471B	PPB	20 Jan 2021 15:31:22	S	Std
2.5 - 1		14765	-	2.50007471B	PPB	20 Jan 2021 15:33:39	S	Std
5.0 - 1	52.5	27471	-	5.00007471B	PPB	20 Jan 2021 15:35:57	S	Std
7.5 - 1	55	43641	-	7.50007471B	PPB	20 Jan 2021 15:38:14	S	Std
10.0 - 1	57.5	56109	-	10.00007471B	PPB	20 Jan 2021 15:40:30	S	Std
ICV77 - 1	ICV77	22366	3.9337	-7471B	PPB	20 Jan 2021 15:43:15	U	SMPL
ICB77 - 1	ICB77	-47	-0.0314	-7471B	PPB	20 Jan 2021 15:45:29	U	SMPL
CCV55 - 1	CCV55	27575	4.8552	-7471B	PPB	20 Jan 2021 15:47:45	U	SMPL
CCB55 - 1	CCB55	-58	-0.0333	-7471B	PPB	20 Jan 2021 15:50:00	U	SMPL
CRA - 1	CRA	1161	0.1824	-7471B	PPB	20 Jan 2021 15:52:15	U	SMPL
HighStd - 1	HighStd	56071	9.8965	-7471B	PPB	20 Jan 2021 15:54:30	U	SMPL
ChkStd - 1	ChkStd	41149	7.2566	-7471B	PPB	20 Jan 2021 15:56:46	U	SMPL
PB134246BL - 1	PBS	-92	-0.0393	-7471B	PPB	20 Jan 2021 15:59:03	U	SMPL
PB134246BS - 1	LCSS	20563	3.6148	-7471B	PPB	20 Jan 2021 16:04:11	U	SMPL
M1169-01 - 1	TP-D	35330	6.2272	-7471B	PPB	20 Jan 2021 16:06:27	U	SMPL
M1177-01 - 1	PILE-1-(0.5-1.0)	5439	0.9392	-7471B	PPB	20 Jan 2021 16:08:43	U	SMPL
M1177-03 - 1	PILE-2-(0.5-1.0)	2131	0.3540	-7471B	PPB	20 Jan 2021 16:11:00	U	SMPL
M1177-03DUP - 1	PILE-2-(0.5-1.0)DUP	2159	0.3589	-7471B	PPB	20 Jan 2021 16:13:17	U	SMPL
M1177-03MS - 1	PILE-2-(0.5-1.0)MS	22078	3.8828	-7471B	PPB	20 Jan 2021 16:15:33	U	SMPL
CCV56 - 1	CCV56	27694	4.8763	-7471B	PPB	20 Jan 2021 16:17:48	U	SMPL
CCB56 - 1	CCB56	-40	-0.0301	-7471B	PPB	20 Jan 2021 16:20:03	U	SMPL
M1177-03MSD - 1	PILE-2-(0.5-1.0)MSD	22301	3.9222	-7471B	PPB	20 Jan 2021 16:22:19	U	SMPL
M1177-03LX5 - 1		372	0.0428	-7471B	PPB	20 Jan 2021 16:24:35	U	SMPL
M1177-03A - 1		23423	4.1207	-7471B	PPB	20 Jan 2021 16:26:51	U	SMPL
CCV57 - 1	CCV57	27674	4.8728	-7471B	PPB	20 Jan 2021 16:29:07	U	SMPL
CCB57 - 1	CCB57	-61	-0.0338	-7471B	PPB	20 Jan 2021 16:31:22	U	SMPL