


LB112909

7470A

INSTRUMENT ID: CV2

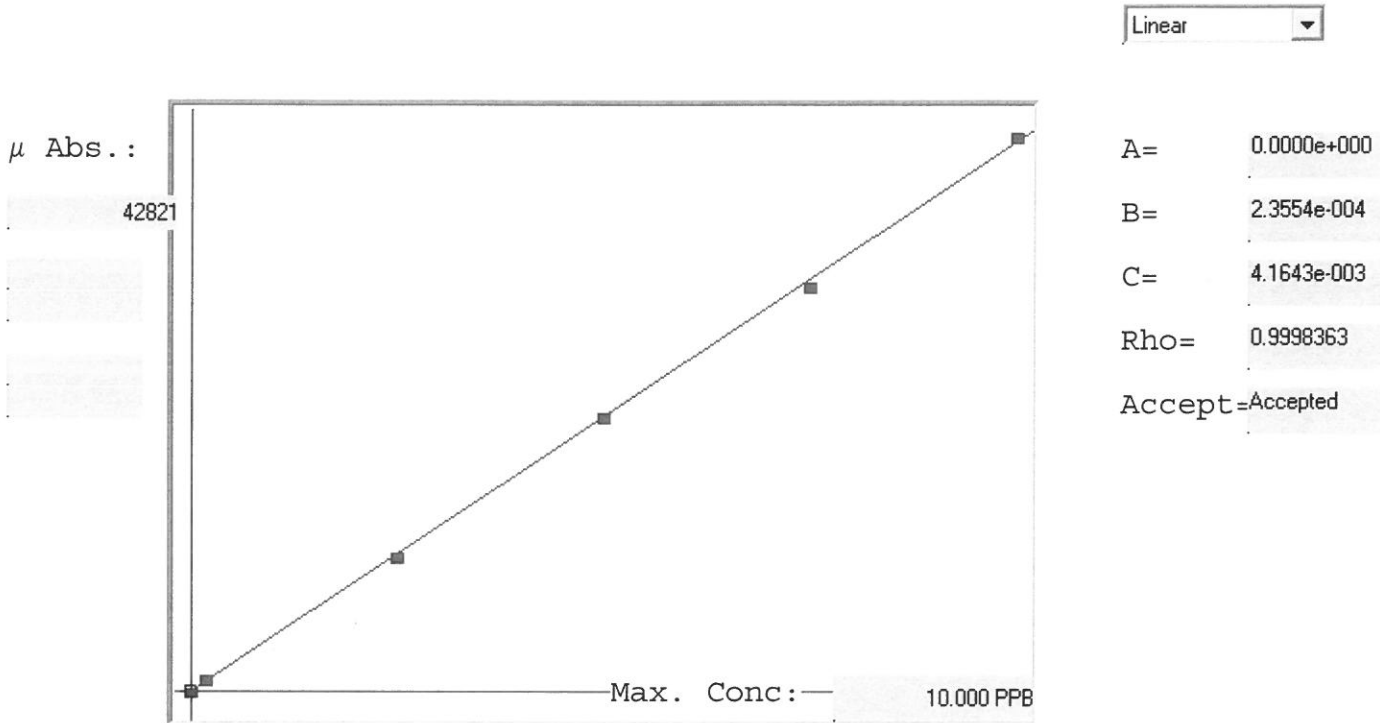

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	0.014	0.014	42	0.000	42					18
0.2	0.200	0.235	0.035	978	0.0 %	978					-1
2.5	2.500	2.471	-0.029	10471	0.0 %	10471					0
5.0	5.000	5.017	0.017	21282	0.0 %	21282					-2
7.5	7.500	7.373	-0.127	31286	0.0 %	31286					0
10.0	10.000	10.090	0.090	42821	0.0 %	42821					

LB112909 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 25 Jan 2021 10:48:57					
Sample ID	Extended ID	µ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	42	-	0.00007470A		PPB	25 Jan 2021 11:03:42	S	Std
0.2 - 1	SO2	978	-	0.20007470A		PPB	25 Jan 2021 11:09:18	S	Std
2.5 - 1	SO2.5	10471	-	2.50007470A		PPB	25 Jan 2021 11:11:35	S	Std
5.0 - 1	SO5	21282	-	5.00007470A		PPB	25 Jan 2021 11:13:52	S	Std
7.5 - 1	SO7.5	31286	-	7.50007470A		PPB	25 Jan 2021 11:16:09	S	Std
10.0 - 1	SO10	42821	-	10.00007470A		PPB	25 Jan 2021 11:20:58	S	Std
ICV81 - 1	ICV81	16225	3.8259	-7470A		PPB	25 Jan 2021 11:23:47	U	SMPL
ICB81 - 1	ICB81	82	0.0235	-7470A		PPB	25 Jan 2021 11:28:35	U	SMPL
CCV71 - 1	CCV71	21408	5.0467	-7470A		PPB	25 Jan 2021 11:30:49	U	SMPL
CCB71 - 1	CCB71	14	0.0075	-7470A		PPB	25 Jan 2021 11:35:39	U	SMPL
CRA - 1	CRA	954	0.2289	-7470A		PPB	25 Jan 2021 11:37:54	U	SMPL
HighStd - 1	HighStd	43809	10.3231	-7470A		PPB	25 Jan 2021 11:40:09	U	SMPL
ChkStd - 1	ChkStd	28991	6.8328	-7470A		PPB	25 Jan 2021 11:42:24	U	SMPL
PB134297BL - 1	PBW	-79	-0.0144	-7470A		PPB	25 Jan 2021 11:44:41	U	SMPL
PB134297BS - 1	LCSW	15196	3.5835	-7470A		PPB	25 Jan 2021 11:49:43	U	SMPL
M1189-06 - 1	41041	824	0.1983	-7470A		PPB	25 Jan 2021 11:52:00	U	SMPL
M1189-07 - 1	41108	1702	0.4051	-7470A		PPB	25 Jan 2021 11:54:16	U	SMPL
M1189-12 - 1	41087-88	83922	19.7715	-7470A		PPB	25 Jan 2021 11:56:35	U	SMPL
M1191-06 - 1	0022-SITE-WATER-043	84	0.0240	-7470A		PPB	25 Jan 2021 12:03:58	U	SMPL
M1191-06DUP - 1	0022-SITE-WATER-043DUP	135	0.0360	-7470A		PPB	25 Jan 2021 12:06:13	U	SMPL
CCV72 - 1	CCV72	20785	4.9000	-7470A		PPB	25 Jan 2021 12:08:29	U	SMPL
CCB72 - 1	CCB72	-114	-0.0227	-7470A		PPB	25 Jan 2021 12:10:44	U	SMPL
M1191-06MS - 1	0022-SITE-WATER-043MS	15995	3.7717	-7470A		PPB	25 Jan 2021 12:13:00	U	SMPL
M1191-06MSD - 1	0022-SITE-WATER-043MSD	15902	3.7498	-7470A		PPB	25 Jan 2021 12:15:16	U	SMPL
M1191-07 - 1	0023-SITE-WATER-044	72	0.0211	-7470A		PPB	25 Jan 2021 12:17:31	U	SMPL
M1191-08 - 1	0024-SITE-WATER-045	132	0.0353	-7470A		PPB	25 Jan 2021 12:19:47	U	SMPL
M1191-09 - 1	0027-SITE-WATER-051	131	0.0350	-7470A		PPB	25 Jan 2021 12:22:03	U	SMPL
M1191-10 - 1	0028-SITE-WATER-052	192	0.0494	-7470A		PPB	25 Jan 2021 12:24:20	U	SMPL
M1212-01 - 1	0021-SITE-WATER-042	107	0.0294	-7470A		PPB	25 Jan 2021 12:26:36	U	SMPL
M1212-02 - 1	0020-FIELD-BLANK	-148	-0.0307	-7470A		PPB	25 Jan 2021 12:28:53	U	SMPL
M1219-01 - 1	IDW-BR2-AQ-012121-01	348	0.0861	-7470A		PPB	25 Jan 2021 12:31:10	U	SMPL
M1219-02 - 1	IDW-BR2-AQ-012121-02	92	0.0258	-7470A		PPB	25 Jan 2021 12:33:25	U	SMPL
CCV73 - 1	CCV73	21095	4.9730	-7470A		PPB	25 Jan 2021 12:35:41	U	SMPL
CCB73 - 1	CCB73	-107	-0.0210	-7470A		PPB	25 Jan 2021 12:37:57	U	SMPL
M1191-06LX5 - 1		56	0.0174	-7470A		PPB	25 Jan 2021 12:40:14	U	SMPL
M1191-06A - 1		15823	3.7312	-7470A		PPB	25 Jan 2021 12:42:30	U	SMPL
M1189-12DLX5 - 1		19475	4.5914	-7470A		PPB	25 Jan 2021 12:44:45	U	SMPL
CCV74 - 1	CCV74	21104	4.9751	-7470A		PPB	25 Jan 2021 12:47:01	U	SMPL
CCB74 - 1	CCB74	-81	-0.0149	-7470A		PPB	25 Jan 2021 12:49:17	U	SMPL