


LB 112936

SFAM01.1

INSTRUMENT ID: CW1

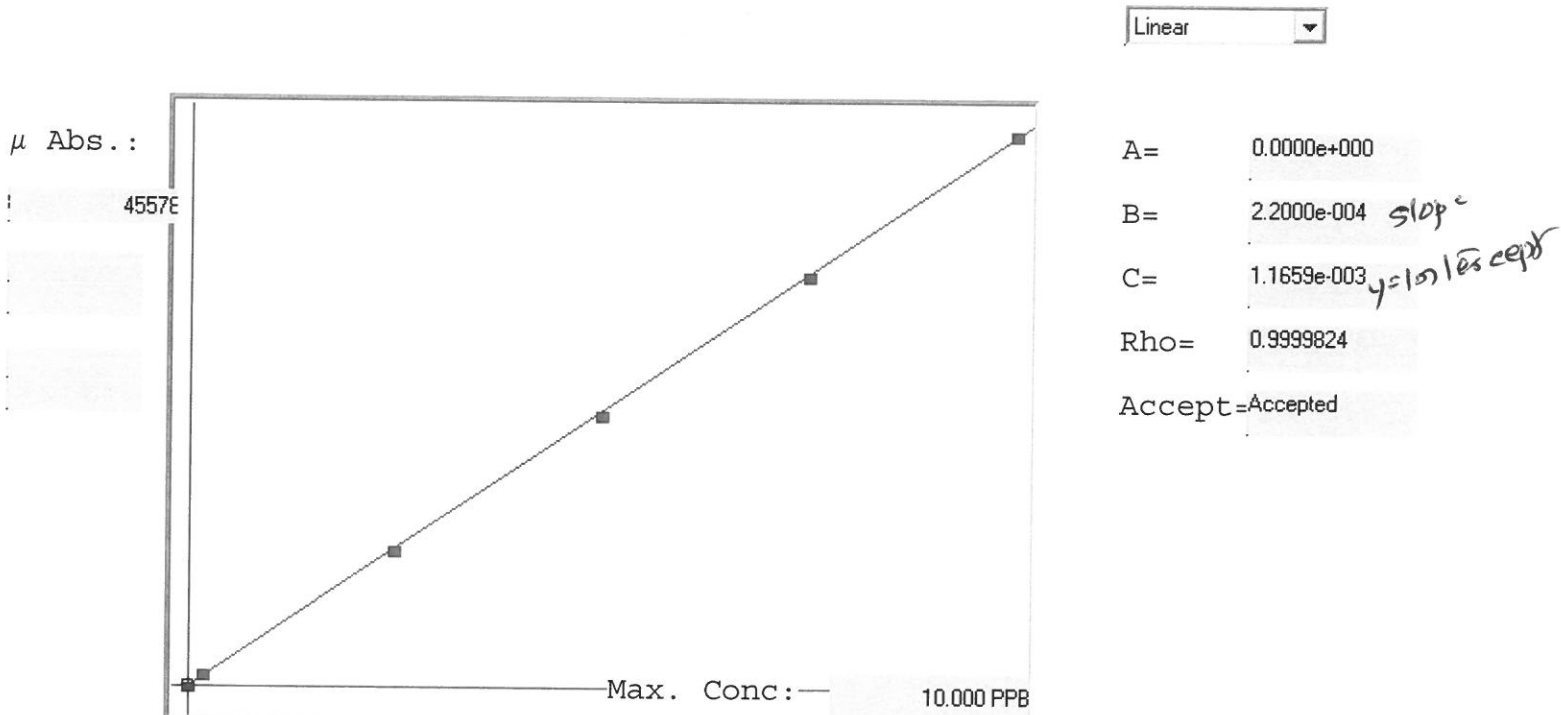

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%OD
0.00	0.000	0.012	0.012	48	0.000	48					118
0.05	0.050					334					101
0.20	0.200	0.216	0.016	978	0.0 %	978					100
2.50	2.500	2.493	-0.007	11325	0.0 %	11325					100
5.00	5.000	4.961	-0.039	22546	0.0 %	22546					100
7.50	7.500	7.489	-0.011	34037	0.0 %	34037					100
10.0	10.000	10.028	0.028	45578	0.0 %	45578					100

LB112936

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	48	-		0 SFAM01.1	PPB	1/27/2021 12:26	Std
	0.2 S01	978	-		0.2 SFAM01.1	PPB	1/27/2021 12:28	Std
	2.5 S02	11325	-		2.5 SFAM01.1	PPB	1/27/2021 12:31	Std
	5 S03	22546	-		5 SFAM01.1	PPB	1/27/2021 12:33	Std
	7.5 S04	34037	-		7.5 SFAM01.1	PPB	1/27/2021 12:35	Std
	10 S05	45578	-		10 SFAM01.1	PPB	1/27/2021 12:45	Std
ICV011	ICV011	17170	3.7786 -		SFAM01.1	PPB	1/27/2021 12:48	SMPL
ICB011	ICB011	-40	-0.0076 -		SFAM01.1	PPB	1/27/2021 12:51	SMPL
CCV093	CCV093	22488	4.9486 -		SFAM01.1	PPB	1/27/2021 12:53	SMPL
CCB093	CCB093	-41	-0.0079 -		SFAM01.1	PPB	1/27/2021 12:55	SMPL
PB134364BL	PBW364	11	0.0036 -		SFAM01.1	PPB	1/27/2021 12:57	SMPL
M1204-07	X2X94	24575	5.4077 -		SFAM01.1	PPB	1/27/2021 13:02	SMPL
M1204-08	X2X94D	24648	5.4238 -		SFAM01.1	PPB	1/27/2021 13:07	SMPL
M1204-09	X2X94S	29019	6.3854 -		SFAM01.1	PPB	1/27/2021 13:09	SMPL
CCV094	CCV094	22494	4.9499 -		SFAM01.1	PPB	1/27/2021 13:13	SMPL
CCB094	CCB094	-38	-0.0072 -		SFAM01.1	PPB	1/27/2021 13:16	SMPL