

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

1/27/2021 14:45

Test: ^{Decent} Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.158	0.0	0.086	
ICB1	-0.089	0.0	0.001	
CCV1	241.220	0.0	0.217	
CCB1	-0.378	0.0	0.000	
PB134365BL	-0.230	0.0	0.001	
M1234-02	-0.399	0.0	0.000	
M1234-02DUP	-0.430	0.0	0.000	
M1236-02	-0.376	0.0	0.000	
M1236-04	-0.360	0.0	0.000	
M1236-06	-0.334	0.0	0.001	
M1236-08	-0.542	0.0	0.000	
M1239-01	-0.363	0.0	0.000	
M1240-01	-0.150	0.0	0.001	
M1240-03	-0.110	0.0	0.001	
CCV2	256.993	0.0	0.231	
CCB2	0.248	0.0	0.001	

N	16
Mean	36.866
SD	86.2335
CV%	233.91

Aquakem v. 7.2AQ1



Results from time period:

Wed Jan 27 13:31:08 2021

Wed Jan 27 14:44:30 2021

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.6259	µg/l	1/27/2021 14:12:06	
5.OPPBCN	A	Reactive CN	P	4.2945	µg/l	1/27/2021 14:12:07	
10PPBCN	A	Reactive CN	P	9.5766	µg/l	1/27/2021 14:12:08	
50PPBCN	A	Reactive CN	P	49.7452	µg/l	1/27/2021 14:12:09	
100PPBCN	A	Reactive CN	P	100.7432	µg/l	1/27/2021 14:12:10	
250PPBCN	A	Reactive CN	P	252.748	µg/l	1/27/2021 14:12:11	
500PPBCN	A	Reactive CN	P	498.5184	µg/l	1/27/2021 14:12:12	
ICV1	S	Reactive CN	P	95.1576	µg/l	1/27/2021 14:39:39	
ICB1	S	Reactive CN	P	-0.0887	µg/l	1/27/2021 14:39:40	
CCV1	S	Reactive CN	P	241.2202	µg/l	1/27/2021 14:39:41	
CCB1	S	Reactive CN	P	-0.3785	µg/l	1/27/2021 14:39:42	
PB134365BL	S	Reactive CN	P	-0.23	µg/l	1/27/2021 14:39:43	
M1234-02	S	Reactive CN	P	-0.3989	µg/l	1/27/2021 14:39:44	
M1234-02DUP	S	Reactive CN	P	-0.4301	µg/l	1/27/2021 14:39:45	
M1236-02	S	Reactive CN	P	-0.3763	µg/l	1/27/2021 14:39:46	
M1236-04	S	Reactive CN	P	-0.3596	µg/l	1/27/2021 14:39:47	
M1236-06	S	Reactive CN	P	-0.3341	µg/l	1/27/2021 14:39:48	
M1236-08	S	Reactive CN	P	-0.5424	µg/l	1/27/2021 14:39:49	
M1239-01	S	Reactive CN	P	-0.3631	µg/l	1/27/2021 14:44:26	
M1240-01	S	Reactive CN	P	-0.1503	µg/l	1/27/2021 14:44:27	
M1240-03	S	Reactive CN	P	-0.1098	µg/l	1/27/2021 14:44:28	
CCV2	S	Reactive CN	P	256.9926	µg/l	1/27/2021 14:44:29	
CCB2	S	Reactive CN	P	0.2479	µg/l	1/27/2021 14:44:30	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

1/27/2021 14:13


Test Total CN

Accepted 1/27/2021 14:13

Factor 1117
Bias 0.001

Coeff. of det. 0.999944

Errors

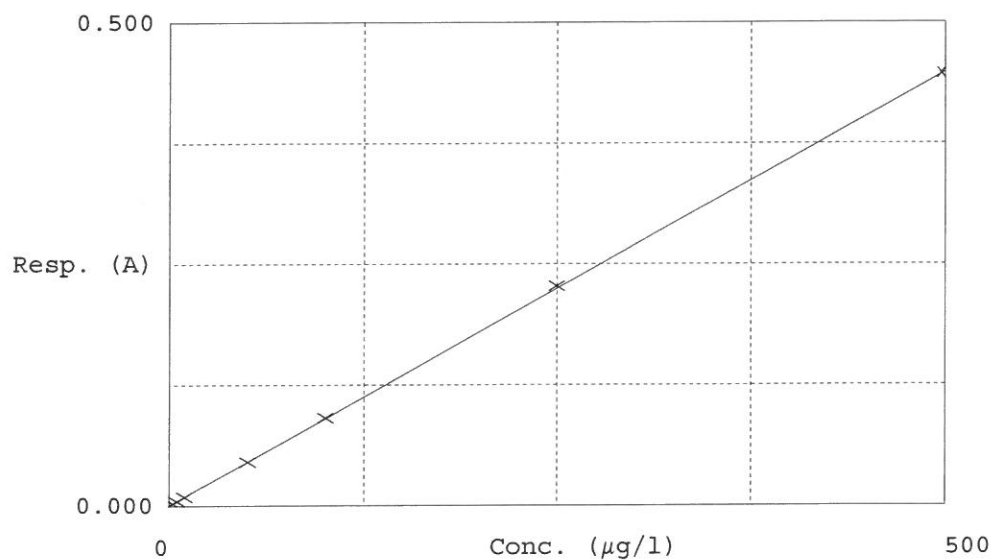

	Calibrator	Response	Calc. con.	Conc.	Errors % D
1	0.0PPBCN	0.000	-0.6259	0.0000	
2	5.0PPBCN	0.005	4.2945	5.0000	
3	10PPBCN	0.009	9.5766	10.0000	
4	50PPBCN	0.045	49.7452	50.0000	
5	100PPBCN	0.091	100.7432	100.0000	
6	250PPBCN	0.227	252.7480	250.0000	
7	500PPBCN	0.447	498.5184	500.0000	

14
5
1
0

M

1/27/21