

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AS Instrument ID : Konelab

2/3/2021 16:45

Test: Phenolics- *mm/v*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.964	0.0	0.112	
ICB1	0.003	0.0	0.007	
CCV1	0.961	0.0	0.111	
CCB1	0.005	0.0	0.007	
PB134409BL	0.003	0.0	0.007	
PB134409BS	0.967	0.0	0.112	
M1278-01	0.004	0.0	0.007	
M1278-01DUP	0.003	0.0	0.007	
M1278-01MS	0.965	0.0	0.112	
M1278-01MSD	0.976	0.0	0.113	
CCV2	0.958	0.0	0.111	
CCB2	0.002	0.0	0.007	

N	12
Mean	0.484
SD	0.5023
CV%	103.73

Aquakem v. 7.2AQ1

Results from time period:

Wed Feb 03 16:13:01 2021

Wed Feb 03 16:43:16 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	0.0047	mg/l	2/3/2021 16:13:01	
0.05PPM	A	Phenolics-	P	0.0483	mg/l	2/3/2021 16:13:02	
0.1PPM	A	Phenolics-	P	0.1003	mg/l	2/3/2021 16:13:03	
0.25PPM	A	Phenolics-	P	0.2584	mg/l	2/3/2021 16:13:04	
0.50PPM	A	Phenolics-	P	0.5037	mg/l	2/3/2021 16:13:05	
1.0PPM	A	Phenolics-	P	0.973	mg/l	2/3/2021 16:13:06	
2.0PPM	A	Phenolics-	P	2.0116	mg/l	2/3/2021 16:13:07	
ICV1	S	Phenolics-	P	0.9636	mg/l	2/3/2021 16:39:17	
ICB1	S	Phenolics-	P	0.0031	mg/l	2/3/2021 16:39:18	
CCV1	S	Phenolics-	P	0.9613	mg/l	2/3/2021 16:39:19	
CCB1	S	Phenolics-	P	0.005	mg/l	2/3/2021 16:39:20	
PB134409BL	S	Phenolics-	P	0.0028	mg/l	2/3/2021 16:39:21	
PB134409BS	S	Phenolics-	P	0.9671	mg/l	2/3/2021 16:39:22	
M1278-01	S	Phenolics-	P	0.0042	mg/l	2/3/2021 16:39:23	
M1278-01DUP	S	Phenolics-	P	0.0026	mg/l	2/3/2021 16:39:24	
M1278-01MS	S	Phenolics-	P	0.9652	mg/l	2/3/2021 16:39:25	
M1278-01MSD	S	Phenolics-	P	0.9756	mg/l	2/3/2021 16:39:26	
CCV2	S	Phenolics-	P	0.9582	mg/l	2/3/2021 16:43:15	
CCB2	S	Phenolics-	P	0.0023	mg/l	2/3/2021 16:43:16	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

2/3/2021 16:16


Test Phenolics-

Accepted 2/3/2021 16:16

Factor 9.157
Bias 0.006

Coeff. of det. 0.999691

Errors

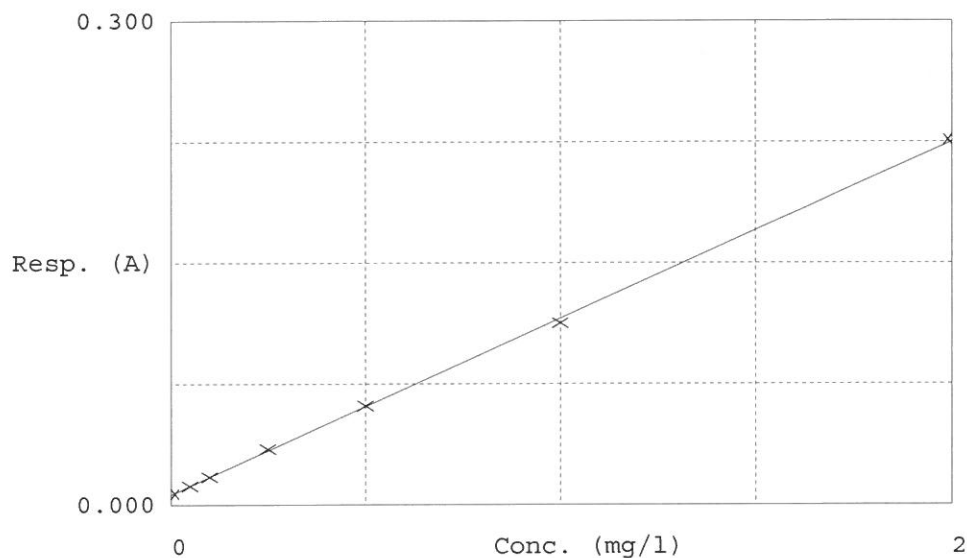

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	0.0047	0.0000	
2	Phenol-2	0.012	0.0483	0.0500	
3	Phenol-2	0.017	0.1003	0.1000	
4	Phenol-2	0.035	0.2584	0.2500	
5	Phenol-2	0.061	0.5037	0.5000	
6	Phenol-2	0.113	0.9730	1.0000	
7	Phenol-2	0.226	2.0116	2.0000	

| 1.0 |

3
0
2
1
3
0

AS

2/3/21