


LB113022

7470A

INSTRUMENT ID: CV2

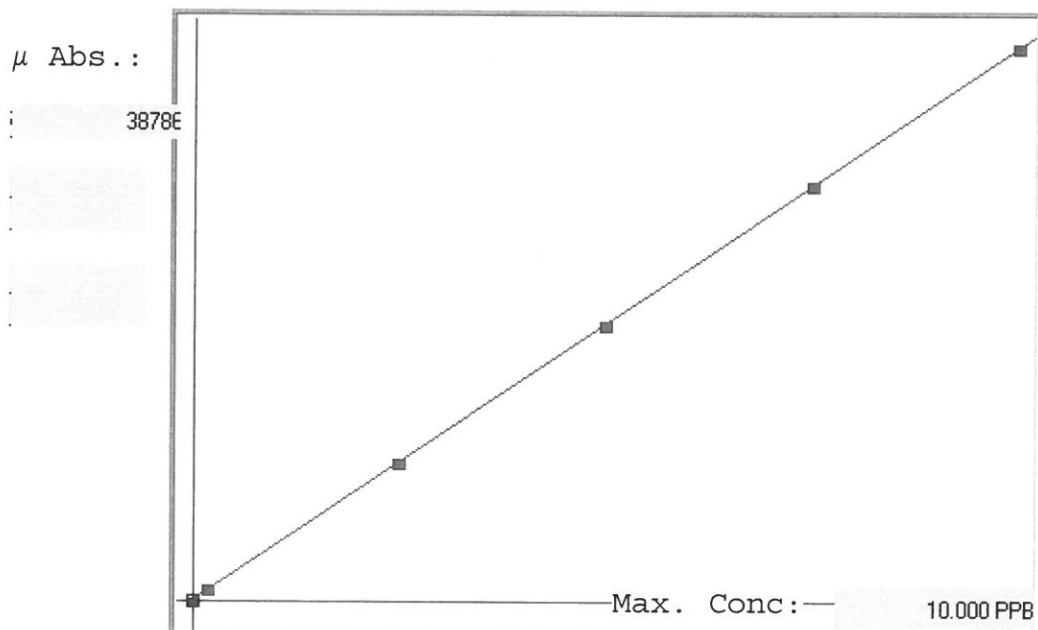

Linear

A= 0.0000e+000

B= 2.5785e-004

C= -1.1922e-002

Rho= 0.9999959

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.005	0.005	67	0.000	67					
0.2	0.200	0.197	-0.003	811	0.0 %	811					
2.5	2.500	2.494	-0.006	9718	0.0 %	9718					
5.0	5.000	4.994	-0.006	19413	0.0 %	19413					
7.5	7.500	7.521	0.021	29214	0.0 %	29214					
10.0	10.000	9.989	-0.011	38786	0.0 %	38786					

1
-2
0
0
0
0

LB113022 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Feb 2021 11:47:07

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	67	-	0.0000	7470A	PPB	04 Feb 2021 11:49:57	S	Std
0.2 - 1	50.2	811	-	0.2000	7470A	PPB	04 Feb 2021 11:52:15	S	Std
2.5 - 1	52.5	9718	-	2.5000	7470A	PPB	04 Feb 2021 11:54:32	S	Std
5.0 - 1	55	19413	-	5.0000	7470A	PPB	04 Feb 2021 11:56:49	S	Std
7.5 - 1	57.5	29214	-	7.5000	7470A	PPB	04 Feb 2021 11:59:05	S	Std
10.0 - 1	510	38786	-	10.0000	7470A	PPB	04 Feb 2021 12:03:59	S	Std
ICV91 - 1	ICV91	15022	3.8615	-	7470A	PPB	04 Feb 2021 12:06:43	U	SMPL
ICB91 - 1	ICB91	-48	-0.0243	-	7470A	PPB	04 Feb 2021 12:08:58	U	SMPL
CCV22 - 1	CCV22	19849	5.1061	-	7470A	PPB	04 Feb 2021 12:11:13	U	SMPL
CCB22 - 1	CCB22	-57	-0.0266	-	7470A	PPB	04 Feb 2021 12:13:28	U	SMPL
CRA - 1	CRA	816	0.1985	-	7470A	PPB	04 Feb 2021 12:15:43	U	SMPL
HighStd - 1	HighStd	37960	9.7760	-	7470A	PPB	04 Feb 2021 12:17:58	U	SMPL
ChkStd - 1	ChkStd	28307	7.2870	-	7470A	PPB	04 Feb 2021 12:20:14	U	SMPL
PB134451BL - 1	PBW	-68	-0.0295	-	7470A	PPB	04 Feb 2021 12:22:31	U	SMPL
PB134451BS - 1	LCSW	14614	3.7563	-	7470A	PPB	04 Feb 2021 12:24:46	U	SMPL
M1267-03 - 1	1-3-DRUMS	28	-0.0047	-	7470A	PPB	04 Feb 2021 12:27:02	U	SMPL
M1267-03DUP - 1	1-3-DRUMSDUP	65	0.0048	-	7470A	PPB	04 Feb 2021 12:29:19	U	SMPL
M1267-03MS - 1	1-3-DRUMSMS	13967	3.5895	-	7470A	PPB	04 Feb 2021 12:31:36	U	SMPL
M1267-03MSD - 1	1-3-DRUMSMSD	15476	3.9786	-	7470A	PPB	04 Feb 2021 12:33:53	U	SMPL
M1293-02 - 1	TEST-PIT-4	1774	0.4455	-	7470A	PPB	04 Feb 2021 12:36:09	U	SMPL
CCV23 - 1	CCV23	20060	5.1605	-	7470A	PPB	04 Feb 2021 12:38:24	U	SMPL
CCB23 - 1	CCB23	-58	-0.0269	-	7470A	PPB	04 Feb 2021 12:40:40	U	SMPL
PB134451TB - 1	PB134410TB	55	0.0023	-	7470A	PPB	04 Feb 2021 12:42:55	U	SMPL
M1267-03LX5 - 1		41	-0.0014	-	7470A	PPB	04 Feb 2021 12:45:11	U	SMPL
M1267-03A - 1		15224	3.9136	-	7470A	PPB	04 Feb 2021 12:47:27	U	SMPL
CCV24 - 1	CCV24	19708	5.0698	-	7470A	PPB	04 Feb 2021 12:49:43	U	SMPL
CCB24 - 1	CCB24	-47	-0.0240	-	7470A	PPB	04 Feb 2021 12:51:59	U	SMPL