

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : Al

Instrument ID : Konelab

2/9/2021 11:02

Test: Ammonia-N

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.029	0.0	0.203	
ICB1	0.011	0.0	0.019	
CCV1	0.989	0.0	0.196	
CCB1	0.006	0.0	0.018	
PB134498BL	0.006	0.0	0.018	
PB134498BS	1.028	0.0	0.203	
M1321-01	0.454	0.0	0.099	
M1321-01DUP	0.445	0.0	0.098	
M1321-01MS	1.406	0.0	0.272	
M1321-01MSD	1.361	0.0	0.264	
M1321-02	0.453	0.0	0.099	
CCV2	1.078	0.0	0.212	
CCB2	0.008	0.0	0.019	

N	13
Mean	0.636
SD	0.5346
CV%	84.00

Aquakem v. 7.2AQ1

Results from time period:

Tue Feb 09 09:49:20 2021

Tue Feb 09 11:01:43 2021

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Ammonia-I	P	0.0129	mg/l	2/9/2021 10:25:30	
0.1PPM	A	Ammonia-I	P	0.1012	mg/l	2/9/2021 10:25:31	
0.2PPM	A	Ammonia-I	P	0.2076	mg/l	2/9/2021 10:25:32	
0.4PPM	A	Ammonia-I	P	0.3988	mg/l	2/9/2021 10:25:33	
1.0PPM	A	Ammonia-I	P	1.0119	mg/l	2/9/2021 10:25:34	
1.3PPM	A	Ammonia-I	P	1.2554	mg/l	2/9/2021 10:25:35	
2.0PPM	A	Ammonia-I	P	2.0455	mg/l	2/9/2021 10:25:36	
ICV1	S	Ammonia-I	P	1.029	mg/l	2/9/2021 10:56:12	
ICB1	S	Ammonia-I	P	0.0106	mg/l	2/9/2021 10:56:13	
CCV1	S	Ammonia-I	P	0.9894	mg/l	2/9/2021 10:56:14	
CCB1	S	Ammonia-I	P	0.0056	mg/l	2/9/2021 10:56:15	
PB134498BL	S	Ammonia-I	P	0.0059	mg/l	2/9/2021 10:56:16	
PB134498BS	S	Ammonia-I	P	1.0277	mg/l	2/9/2021 10:56:17	
M1321-01	S	Ammonia-I	P	0.4539	mg/l	2/9/2021 10:56:18	
M1321-01DUP	S	Ammonia-I	P	0.4446	mg/l	2/9/2021 10:56:19	
M1321-01MS	S	Ammonia-I	P	1.4057	mg/l	2/9/2021 10:56:20	
M1321-01MSD	S	Ammonia-I	P	1.3615	mg/l	2/9/2021 10:56:21	
M1321-02	S	Ammonia-I	P	0.4532	mg/l	2/9/2021 10:56:23	
CCV2	S	Ammonia-I	P	1.0784	mg/l	2/9/2021 11:01:41	
CCB2	S	Ammonia-I	P	0.0083	mg/l	2/9/2021 11:01:42	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AA

Instrument ID : Konelab

2/9/2021 10:28

Test Ammonia-N


Accepted 2/9/2021 10:28

Factor 5.529

Bias 0.017

Coeff. of det. 0.997479

Errors

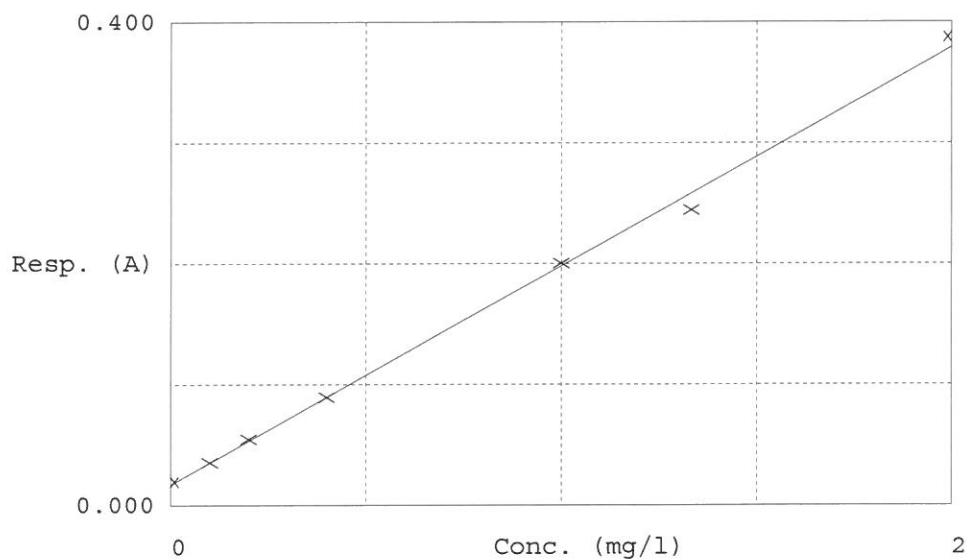

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.020	0.0129	0.0000	
2	NH3-2PPM	0.036	0.1012	0.1000	
3	NH3-2PPM	0.055	0.2076	0.2000	
4	NH3-2PPM	0.089	0.3988	0.4000	
5	NH3-2PPM	0.200	1.0119	1.0000	
6	NH3-2PPM	0.244	1.2554	1.3333	
7	NH3-2PPM	0.387	2.0455	2.0000	

1/1.01

1
4
0
1
6
2

AL

2/9/21