


LB113093

7471B

INSTRUMENT ID: CV1

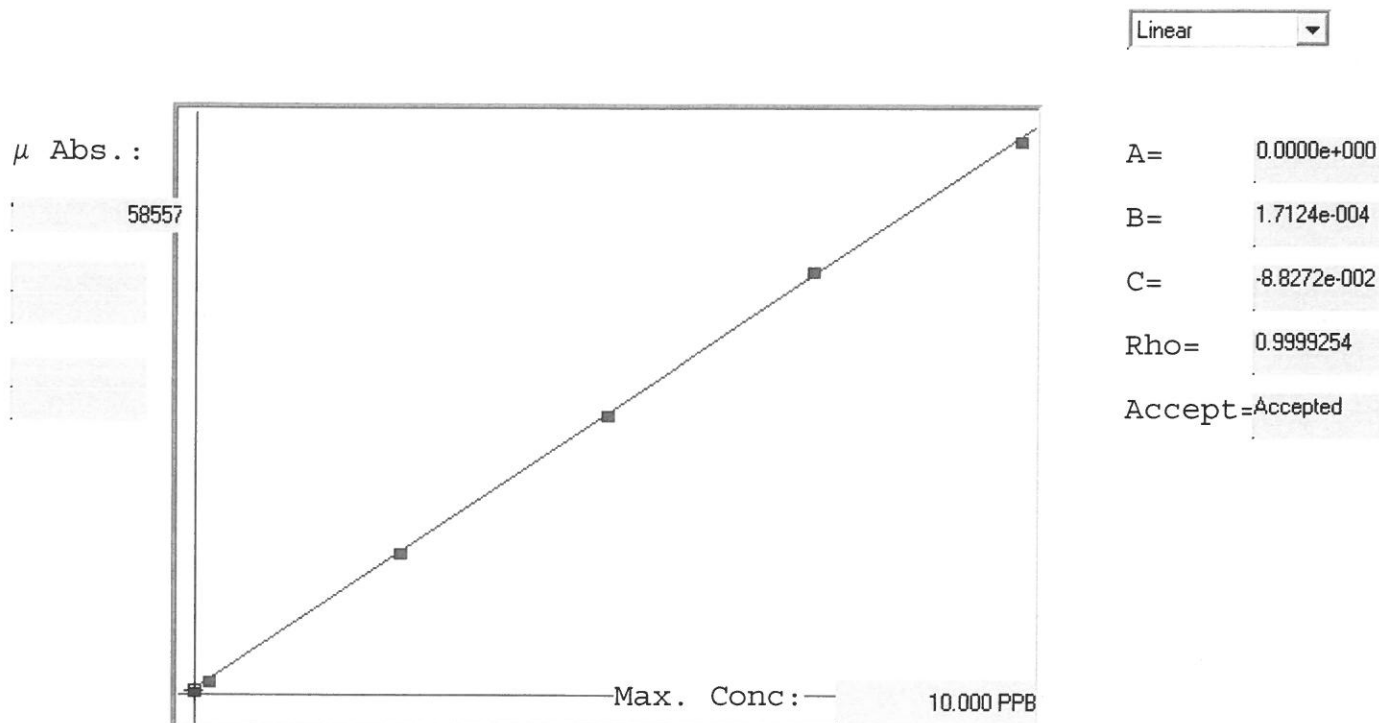

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.012	0.012	588	0.000	588				
0.2	0.200	0.176	-0.024	1544	0.0 %	1544				
2.5	2.500	2.492	-0.008	15066	0.0 %	15066				
5.0	5.000	4.993	-0.007	29674	0.0 %	29674				
7.5	7.500	7.587	0.087	44824	0.0 %	44824				
10.0	10.000	9.939	-0.061	58557	0.0 %	58557				

900
-12
0
0
1
1

LB113093 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 11 Feb 2021 09:05:25					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	588	-	0.0000	7471B	PPB	11 Feb 2021 09:10:12	S	Std
0.2 - 1	50.2	1544	-	0.2000	7471B	PPB	11 Feb 2021 09:12:30	S	Std
2.5 - 1	52.5	15066	-	2.5000	7471B	PPB	11 Feb 2021 09:14:48	S	Std
5.0 - 1	55	29674	-	5.0000	7471B	PPB	11 Feb 2021 09:17:05	S	Std
7.5 - 1	57.5	44824	-	7.5000	7471B	PPB	11 Feb 2021 09:19:22	S	Std
10.0 - 1	510	58557	-	10.0000	7471B	PPB	11 Feb 2021 09:21:38	S	Std
ICV98 - 1	ICV98	22550	3.7732	-	7471B	PPB	11 Feb 2021 09:24:24	U	SMPL
ICB98 - 1	ICB98	486	-0.0050	-	7471B	PPB	11 Feb 2021 09:26:39	U	SMPL
CCV57 - 1	CCV57	29793	5.0135	-	7471B	PPB	11 Feb 2021 09:28:55	U	SMPL
CCB57 - 1	CCB57	497	-0.0032	-	7471B	PPB	11 Feb 2021 09:31:10	U	SMPL
CRA - 1	CRA	1554	0.1778	-	7471B	PPB	11 Feb 2021 09:33:26	U	SMPL
HighStd - 1	HighStd	58188	9.8760	-	7471B	PPB	11 Feb 2021 09:35:41	U	SMPL
ChkStd - 1	ChkStd	43010	7.2768	-	7471B	PPB	11 Feb 2021 09:37:57	U	SMPL
PB134569BL - 1	PBS	433	-0.0141	-	7471B	PPB	11 Feb 2021 09:40:14	U	SMPL
PB134569BS - 1	LCSS	22362	3.7410	-	7471B	PPB	11 Feb 2021 09:42:31	U	SMPL
M1338-01 - 1	OK-02-020921	1211	0.1191	-	7471B	PPB	11 Feb 2021 09:44:48	U	SMPL
M1345-01 - 1	NB-07-020921	2435	0.3287	-	7471B	PPB	11 Feb 2021 09:47:04	U	SMPL
M1345-01DUP - 1	NB-07-020921DUP	2695	0.3732	-	7471B	PPB	11 Feb 2021 09:49:22	U	SMPL
M1345-01MS - 1	NB-07-020921MS	25129	4.2149	-	7471B	PPB	11 Feb 2021 09:51:38	U	SMPL
M1345-01MSD - 1	NB-07-020921MSD	24265	4.0669	-	7471B	PPB	11 Feb 2021 09:53:54	U	SMPL
CCV58 - 1	CCV58	29697	4.9971	-	7471B	PPB	11 Feb 2021 09:56:09	U	SMPL
CCB58 - 1	CCB58	502	-0.0023	-	7471B	PPB	11 Feb 2021 09:58:25	U	SMPL
M1346-01 - 1	EO-03-020921	7899	1.2644	-	7471B	PPB	11 Feb 2021 10:00:41	U	SMPL
M1347-01 - 1	OR-03-020921	3101	0.4427	-	7471B	PPB	11 Feb 2021 10:02:57	U	SMPL
M1348-01 - 1	AS-CON	800	0.0487	-	7471B	PPB	11 Feb 2021 10:05:12	U	SMPL
M1380-01 - 1	PM-WCS-C-001	678	0.0278	-	7471B	PPB	11 Feb 2021 10:07:29	U	SMPL
M1380-02 - 1	PM-WCS-C-002	522	0.0011	-	7471B	PPB	11 Feb 2021 10:09:45	U	SMPL
M1345-01LX5 - 1		834	0.0545	-	7471B	PPB	11 Feb 2021 10:12:01	U	SMPL
M1345-01A - 1		24264	4.0667	-	7471B	PPB	11 Feb 2021 10:14:18	U	SMPL
CCV59 - 1	CCV59	28707	4.8276	-	7471B	PPB	11 Feb 2021 10:16:35	U	SMPL
CCB59 - 1	CCB59	485	-0.0052	-	7471B	PPB	11 Feb 2021 10:18:53	U	SMPL