


LB115168

7470A

INSTRUMENT ID: CV2

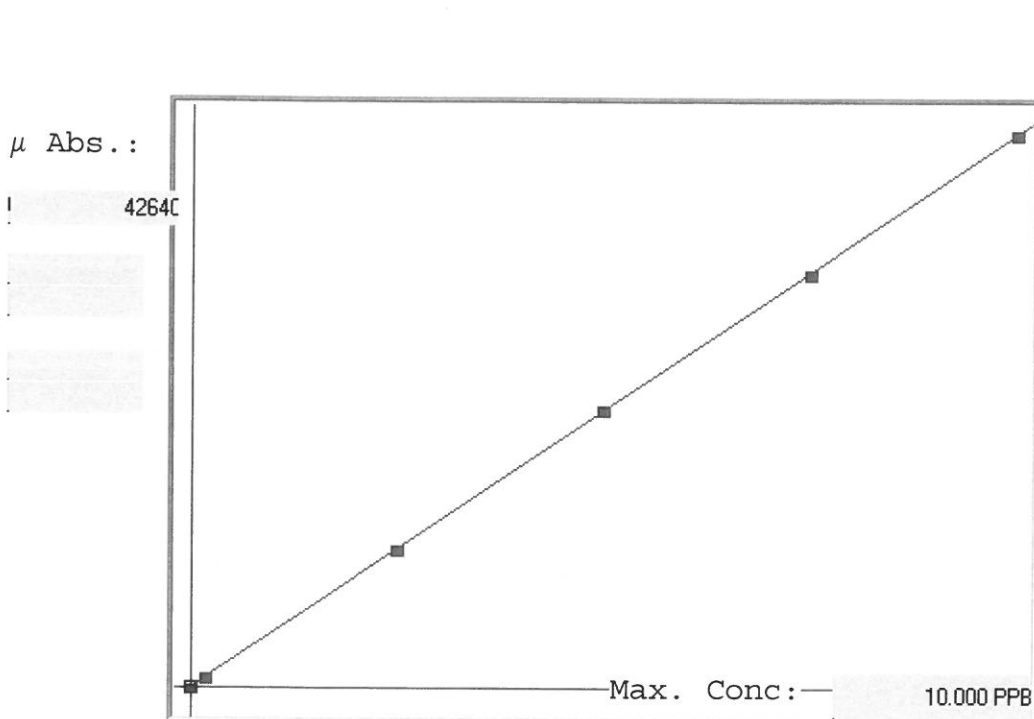

Linear

A= 0.0000e+000

B= 2.3441e-004

C= -3.6792e-003

Rho= 0.9999924

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.001	0.001	18	0.000	18					
0.2	0.200	0.193	-0.007	840	0.0 %	840					-4
2.5	2.500	2.489	-0.011	10636	0.0 %	10636					0
5.0	5.000	5.031	0.031	21479	0.0 %	21479					1
7.5	7.500	7.494	-0.006	31986	0.0 %	31986					0
10.0	10.000	9.991	-0.009	42640	0.0 %	42640					0

LB113168 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Feb 2021 11:56:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1		18	-	0.0000	7470A	PPB	17 Feb 2021 11:57:41	S	Std
0.2 - 1		840	-	0.2000	7470A	PPB	17 Feb 2021 11:59:59	S	Std
2.5 - 1		10636	-	2.5000	7470A	PPB	17 Feb 2021 12:02:16	S	Std
5.0 - 1		21479	-	5.0000	7470A	PPB	17 Feb 2021 12:04:33	S	Std
7.5 - 1		31986	-	7.5000	7470A	PPB	17 Feb 2021 12:06:49	S	Std
10.0 - 1		42640	-	10.0000	7470A	PPB	17 Feb 2021 12:09:05	S	Std
ICV06 - 1	ICV06	16843	3.9445	-	7470A	PPB	17 Feb 2021 12:11:47	U	SMPL
ICB06 - 1	ICB06	-4	-0.0046	-	7470A	PPB	17 Feb 2021 12:14:03	U	SMPL
CCV91 - 1	CCV91	21313	4.9923	-	7470A	PPB	17 Feb 2021 12:16:17	U	SMPL
CCB91 - 1	CCB91	-32	-0.0112	-	7470A	PPB	17 Feb 2021 12:18:33	U	SMPL
CRA - 1	CRA	782	0.1796	-	7470A	PPB	17 Feb 2021 12:20:48	U	SMPL
HighStd - 1	HighStd	41946	9.8288	-	7470A	PPB	17 Feb 2021 12:23:03	U	SMPL
ChkStd - 1	ChkStd	29658	6.9484	-	7470A	PPB	17 Feb 2021 12:25:18	U	SMPL
PB134696BL - 1	PBW	-39	-0.0128	-	7470A	PPB	17 Feb 2021 12:27:34	U	SMPL
PB134696BS - 1	LCSW	16580	3.8828	-	7470A	PPB	17 Feb 2021 12:29:50	U	SMPL
M1425-06 - 1	SLUDGE-COMP	-11	-0.0063	-	7470A	PPB	17 Feb 2021 12:32:07	U	SMPL
M1425-06DUP - 1	SLUDGE-COMPDUP	18	0.0005	-	7470A	PPB	17 Feb 2021 12:34:23	U	SMPL
M1425-06MS - 1	SLUDGE-COMPMS	17012	3.9841	-	7470A	PPB	17 Feb 2021 12:36:40	U	SMPL
M1425-06MSD - 1	SLUDGE-COMPMSD	16980	3.9766	-	7470A	PPB	17 Feb 2021 12:38:57	U	SMPL
PB134697BL - 1	PBW	-27	-0.0100	-	7470A	PPB	17 Feb 2021 12:41:12	U	SMPL
CCV92 - 1	CCV92	21116	4.9461	-	7470A	PPB	17 Feb 2021 12:43:28	U	SMPL
CCB92 - 1	CCB92	-30	-0.0107	-	7470A	PPB	17 Feb 2021 12:45:43	U	SMPL
PB134697BS - 1	LCSW	17245	4.0387	-	7470A	PPB	17 Feb 2021 12:47:58	U	SMPL
M1425-12 - 1	WATER-COMP	-5	-0.0049	-	7470A	PPB	17 Feb 2021 12:50:14	U	SMPL
M1425-12DUP - 1	WATER-COMPDUP	31	0.0036	-	7470A	PPB	17 Feb 2021 12:52:29	U	SMPL
M1425-12MS - 1	WATER-COMPMS	17108	4.0066	-	7470A	PPB	17 Feb 2021 12:54:45	U	SMPL
M1425-12MSD - 1	WATER-COMPMSD	16971	3.9745	-	7470A	PPB	17 Feb 2021 12:57:01	U	SMPL
M1425-13 - 1	41061	-12	-0.0065	-	7470A	PPB	17 Feb 2021 12:59:17	U	SMPL
PB134698BL - 1	PBW	32	0.0038	-	7470A	PPB	17 Feb 2021 13:01:33	U	SMPL
PB134698BS - 1	LCSW	16702	3.9114	-	7470A	PPB	17 Feb 2021 13:03:50	U	SMPL
M1431-01 - 1	IDW-BR2-AQ-BR-021621	-65	-0.0189	-	7470A	PPB	17 Feb 2021 13:06:07	U	SMPL
CCV93 - 1	CCV93	20741	4.8582	-	7470A	PPB	17 Feb 2021 13:08:22	U	SMPL
CCB93 - 1	CCB93	-35	-0.0119	-	7470A	PPB	17 Feb 2021 13:10:38	U	SMPL
M1432-03 - 1	GWBR2-SC-93-021621	-22	-0.0088	-	7470A	PPB	17 Feb 2021 13:12:55	U	SMPL
M1432-03DUP - 1	GWBR2-SC-93-021621DUP	-15	-0.0072	-	7470A	PPB	17 Feb 2021 13:15:10	U	SMPL
M1432-03MS - 1	GWBR2-SC-93-021621MS	15663	3.6679	-	7470A	PPB	17 Feb 2021 13:17:26	U	SMPL
M1432-03MSD - 1	GWBR2-SC-93-021621MSD	15864	3.7150	-	7470A	PPB	17 Feb 2021 13:19:42	U	SMPL
PB134696TB - 1	PB134676TB	-37	-0.0124	-	7470A	PPB	17 Feb 2021 13:21:57	U	SMPL
PB134697TB - 1	PB134767TB	2	-0.0032	-	7470A	PPB	17 Feb 2021 13:24:13	U	SMPL
CCV94 - 1	CCV94	20921	4.9004	-	7470A	PPB	17 Feb 2021 13:26:31	U	SMPL
CCB94 - 1	CCB94	-36	-0.0121	-	7470A	PPB	17 Feb 2021 13:28:47	U	SMPL
M1425-06LX5 - 1		27	0.0026	-	7470A	PPB	17 Feb 2021 13:31:05	U	SMPL
M1425-06A - 1		16085	3.7668	-	7470A	PPB	17 Feb 2021 13:33:22	U	SMPL
M1425-12LX5 - 1		-42	-0.0135	-	7470A	PPB	17 Feb 2021 13:35:38	U	SMPL
M1425-12A - 1		16657	3.9009	-	7470A	PPB	17 Feb 2021 13:37:54	U	SMPL
M1432-03LX5 - 1		-32	-0.0112	-	7470A	PPB	17 Feb 2021 13:40:10	U	SMPL
M1432-03A - 1		16103	3.7710	-	7470A	PPB	17 Feb 2021 13:42:25	U	SMPL
CCV95 - 1	CCV95	20304	4.7557	-	7470A	PPB	17 Feb 2021 13:44:41	U	SMPL
CCB95 - 1	CCB95	-51	-0.0156	-	7470A	PPB	17 Feb 2021 13:46:57	U	SMPL