

LB13200

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : AM Instrument ID : Konelab

2/19/2021 13:43

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	94.428	0.0	0.094	
ICB1	-0.194	0.0	0.001	
CCV1	240.950	0.0	0.239	
CCB1	-0.205	0.0	0.001	
PB134736BL	-0.337	0.0	0.001	
M1434-02	-0.110	0.0	0.001	
M1434-02DUP	-0.398	0.0	0.001	
M1436-01	-0.633	0.0	0.000	
M1436-03	-0.509	0.0	0.000	
M1437-01	-0.492	0.0	0.001	
M1437-03	-0.360	0.0	0.001	
CCV2	249.894	0.0	0.248	
CCB2	-0.264	0.0	0.001	

N	13
Mean	44.751
SD	92.8201
CV%	207.41

Aquakem v. 7.2AQ1

Results from time period:

Fri Feb 19 13:13:42 2021

Fri Feb 19 13:41:49 2021

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	-0.7264	µg/l	2/19/2021 10:50:40
5.OPPBCN	A	Reactive CN	P	4.0156	µg/l	2/19/2021 10:50:41
10PPBCN	A	Reactive CN	P	9.4347	µg/l	2/19/2021 10:50:42
50PPBCN	A	Reactive CN	P	50.3783	µg/l	2/19/2021 10:50:43
100PPBCN	A	Reactive CN	P	99.9796	µg/l	2/19/2021 10:50:44
250PPBCN	A	Reactive CN	P	253.8615	µg/l	2/19/2021 10:50:45
500PPBCN	A	Reactive CN	P	498.0566	µg/l	2/19/2021 10:50:46
ICV1	S	Reactive CN	P	94.4276	µg/l	2/19/2021 13:13:43
ICB1	S	Reactive CN	P	-0.1937	µg/l	2/19/2021 13:13:45
CCV1	S	Reactive CN	P	240.9498	µg/l	2/19/2021 13:13:46
CCB1	S	Reactive CN	P	-0.2049	µg/l	2/19/2021 13:13:48
PB134736BL	S	Reactive CN	P	-0.3372	µg/l	2/19/2021 13:13:50
M1434-02	S	Reactive CN	P	-0.1102	µg/l	2/19/2021 13:13:51
M1434-02DUP	S	Reactive CN	P	-0.3978	µg/l	2/19/2021 13:13:52
M1436-01	S	Reactive CN	P	-0.6326	µg/l	2/19/2021 13:19:53
M1436-03	S	Reactive CN	P	-0.5089	µg/l	2/19/2021 13:19:54
M1437-01	S	Reactive CN	P	-0.4924	µg/l	2/19/2021 13:41:43
M1437-03	S	Reactive CN	P	-0.36	µg/l	2/19/2021 13:41:44
CCV2	S	Reactive CN	P	249.8938	µg/l	2/19/2021 13:41:47
CCB2	S	Reactive CN	P	-0.2644	µg/l	2/19/2021 13:41:48

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

2/19/2021 10:54


Test Total CN

Accepted 2/19/2021 10:54

Factor 1013
Bias 0.001

Coeff. of det. 0.999900

Errors

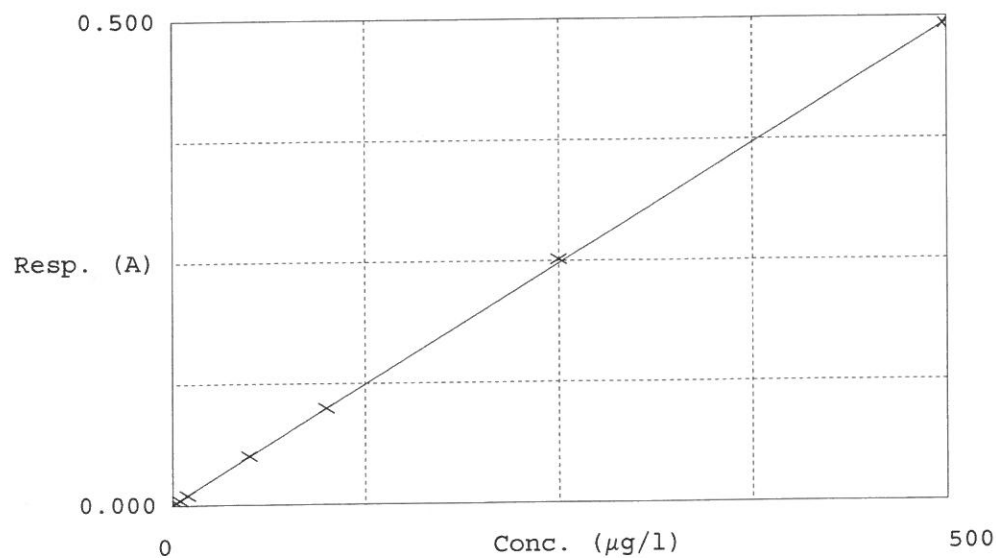

	Calibrator	Response	Calc. con.	Conc.	Errors	%DI
1	0.0PPBCN	0.000	-0.7264	0.0000		
2	5.0PPBCN	0.005	4.0156	5.0000		
3	10PPBCN	0.010	9.4347	10.0000		
4	50PPBCN	0.051	50.3783	50.0000		
5	100PPBCN	0.100	99.9796	100.0000		
6	250PPBCN	0.252	253.8615	250.0000		
7	500PPBCN	0.493	498.0566	500.0000		

20
6
1
0
1
0

02/19/2021