


LB113236

7470A

INSTRUMENT ID: CV1

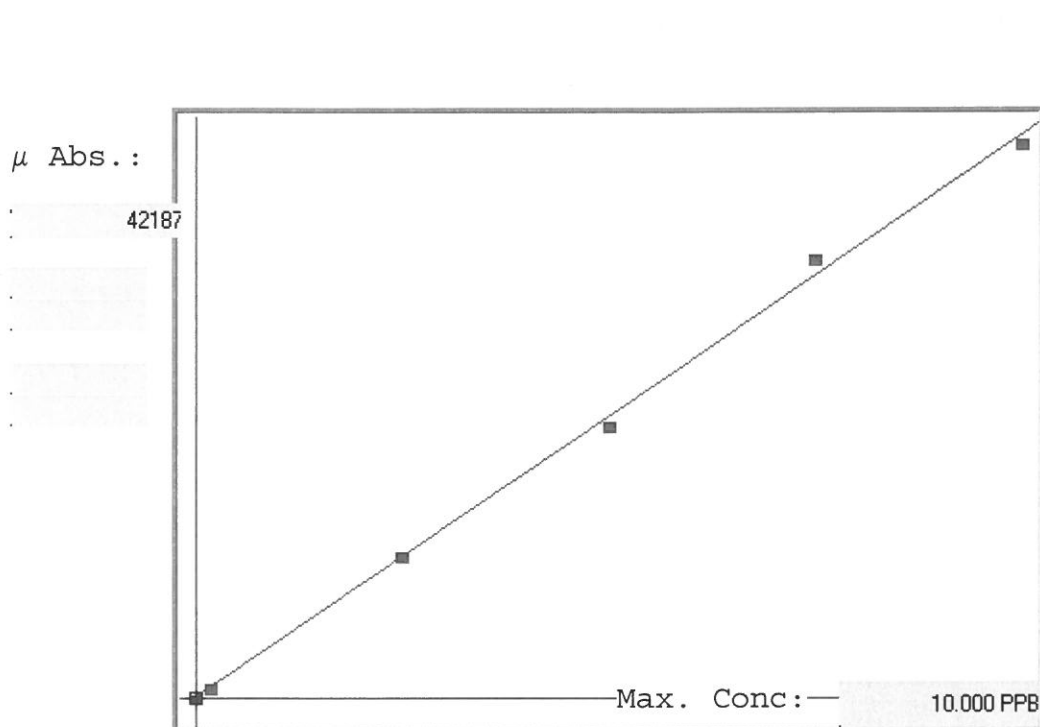

Linear

A= 0.0000e+000

B= 2.3333e-004

C= -1.1305e-002

Rho= 0.9991812

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.005	-0.005	27	0.000	27					-
0.2	0.200	0.190	-0.010	864	0.0 %	864					-5
2.5	2.500	2.536	0.036	10917	0.0 %	10917					1
5.0	5.000	4.857	-0.143	20865	0.0 %	20865					-3
7.5	7.500	7.789	0.289	33432	0.0 %	33432					4
10.0	10.000	9.832	-0.168	42187	0.0 %	42187					-2

LB113236 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 Feb 2021 10:36:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	27	-	0.0000	7470A	PPB	24 Feb 2021 10:41:18	S	Std
0.2 - 1	51.2	864	-	0.2000	7470A	PPB	24 Feb 2021 10:43:35	S	Std
2.5 - 1	52.5	10917	-	2.5000	7470A	PPB	24 Feb 2021 10:45:53	S	Std
5.0 - 1	55	20865	-	5.0000	7470A	PPB	24 Feb 2021 10:48:10	S	Std
7.5 - 1	57.5	33432	-	7.5000	7470A	PPB	24 Feb 2021 10:50:26	S	Std
10.0 - 1	518	42187	-	10.0000	7470A	PPB	24 Feb 2021 10:52:42	S	Std
ICV11 - 1	ICV11	16356	3.8050	-	7470A	PPB	24 Feb 2021 10:55:33	U	SMPL
ICB11 - 1	ICB11	-59	-0.0251	-	7470A	PPB	24 Feb 2021 10:57:47	U	SMPL
CCV24 - 1	CCV24	21060	4.9026	-	7470A	PPB	24 Feb 2021 11:00:03	U	SMPL
CCB24 - 1	CCB24	-66	-0.0267	-	7470A	PPB	24 Feb 2021 11:02:18	U	SMPL
CRA - 1	CRA	816	0.1791	-	7470A	PPB	24 Feb 2021 11:04:33	U	SMPL
HighStd - 1	HighStd	39819	9.2797	-	7470A	PPB	24 Feb 2021 11:06:48	U	SMPL
ChkStd - 1	ChkStd	29330	6.8323	-	7470A	PPB	24 Feb 2021 11:09:50	U	SMPL
PB134787BL - 1	PBW	-60	-0.0253	-	7470A	PPB	24 Feb 2021 11:12:06	U	SMPL
PB134787BS - 1	LCSW	14644	3.4056	-	7470A	PPB	24 Feb 2021 11:14:22	U	SMPL
M1461-01 - 1	31155	-7	-0.0129	-	7470A	PPB	24 Feb 2021 11:16:38	U	SMPL
M1461-01DUP - 1	31155DUP	32	-0.0038	-	7470A	PPB	24 Feb 2021 11:18:55	U	SMPL
M1461-01MS - 1	31155MS	16447	3.8263	-	7470A	PPB	24 Feb 2021 11:21:12	U	SMPL
M1461-01MSD - 1	31155MSD	15827	3.6816	-	7470A	PPB	24 Feb 2021 11:23:29	U	SMPL
M1464-01 - 1	2-22A	-26	-0.0174	-	7470A	PPB	24 Feb 2021 11:25:44	U	SMPL
CCV25 - 1	CCV25	21097	4.9113	-	7470A	PPB	24 Feb 2021 11:27:59	U	SMPL
CCB25 - 1	CCB25	-48	-0.0225	-	7470A	PPB	24 Feb 2021 11:30:15	U	SMPL
M1464-02 - 1	2-22B	13	-0.0083	-	7470A	PPB	24 Feb 2021 11:32:30	U	SMPL
M1464-03 - 1	2-22C	43	-0.0013	-	7470A	PPB	24 Feb 2021 11:35:22	U	SMPL
M1464-04 - 1	2-22D	39	-0.0022	-	7470A	PPB	24 Feb 2021 11:37:37	U	SMPL
M1464-05 - 1	2-22E	37	-0.0027	-	7470A	PPB	24 Feb 2021 11:39:53	U	SMPL
PB134787TB - 1	PB134774TB	55	0.0015	-	7470A	PPB	24 Feb 2021 11:42:09	U	SMPL
M1461-01LX5 - 1		23	-0.0059	-	7470A	PPB	24 Feb 2021 11:44:25	U	SMPL
M1461-01A - 1		16263	3.7833	-	7470A	PPB	24 Feb 2021 11:46:42	U	SMPL
CCV26 - 1	CCV26	21041	4.8982	-	7470A	PPB	24 Feb 2021 11:48:59	U	SMPL
CCB26 - 1	CCB26	-40	-0.0206	-	7470A	PPB	24 Feb 2021 11:51:16	U	SMPL