


LB 113 273

7470A

INSTRUMENT ID: CVZ

Linear

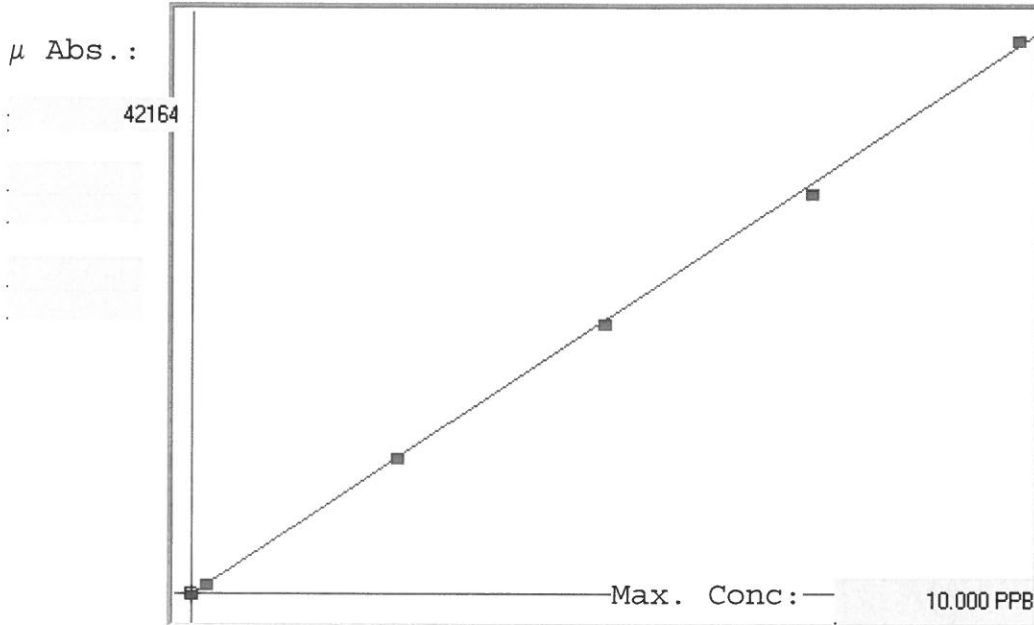

A= 0.0000e+000

B= 2.3943e-004

C= 2.7473e-002

Rho= 0.9997585

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%ob
0.0	0.000	0.037	0.037	40	0.000	40					9
0.2	0.200	0.218	0.018	797	0.0 %	797					0
2.5	2.500	2.508	0.008	10362	0.0 %	10362					-1
5.0	5.000	4.957	-0.043	20589	0.0 %	20589					-2
7.5	7.500	7.356	-0.144	30608	0.0 %	30608					1
10.0	10.000	10.123	0.123	42164	0.0 %	42164					

LB113273 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 26 Feb 2021 09:53:02				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	30	40	-	0.00007470A	PPB	26 Feb 2021 09:53:23	S	Std
0.2 - 1	50.2	797	-	0.20007470A	PPB	26 Feb 2021 09:55:41	S	Std
2.5 - 1	52.5	10362	-	2.50007470A	PPB	26 Feb 2021 09:57:59	S	Std
5.0 - 1	55	20589	-	5.00007470A	PPB	26 Feb 2021 10:00:15	S	Std
7.5 - 1	57.5	30608	-	7.50007470A	PPB	26 Feb 2021 10:02:32	S	Std
10.0 - 1	510	42164	-	10.00007470A	PPB	26 Feb 2021 10:04:48	S	Std
ICV15 - 1	ICV15	15775	3.8045	-7470A	PPB	26 Feb 2021 10:08:13	U	SMPL
ICB15 - 1	ICB15	-25	0.0215	-7470A	PPB	26 Feb 2021 10:10:28	U	SMPL
CCV36 - 1	CCV36	20861	5.0223	-7470A	PPB	26 Feb 2021 10:12:43	U	SMPL
CCB36 - 1	CCB36	-24	0.0217	-7470A	PPB	26 Feb 2021 10:14:58	U	SMPL
CRA - 1	CRA	790	0.2166	-7470A	PPB	26 Feb 2021 10:17:14	U	SMPL
HighStd - 1	HighStd	41035	9.8526	-7470A	PPB	26 Feb 2021 10:19:29	U	SMPL
ChkStd - 1	ChkStd	27724	6.6655	-7470A	PPB	26 Feb 2021 10:21:44	U	SMPL
PB134819BL - 1	PBW	-88	0.0064	-7470A	PPB	26 Feb 2021 10:24:00	U	SMPL
PB134819BS - 1	LCSW	15500	3.7387	-7470A	PPB	26 Feb 2021 10:26:17	U	SMPL
M1471-01 - 1	TREMONT-DRUM-PPE-WASTE	-32	0.0198	-7470A	PPB	26 Feb 2021 10:28:33	U	SMPL
M1471-02 - 1	TREMONT-DRUM-POLY-WASTE	26	0.0337	-7470A	PPB	26 Feb 2021 10:32:43	U	SMPL
M1472-04 - 1	COMPOSITE-01(TP2-TP1)	42	0.0375	-7470A	PPB	26 Feb 2021 10:35:00	U	SMPL
M1472-05 - 1	TEST-PIT-02-EXTRA	33	0.0354	-7470A	PPB	26 Feb 2021 10:37:17	U	SMPL
M1475-02 - 1	WA-CON	152	0.0639	-7470A	PPB	26 Feb 2021 10:39:32	U	SMPL
CCV37 - 1	CCV37	20705	4.9849	-7470A	PPB	26 Feb 2021 10:41:48	U	SMPL
CCB37 - 1	CCB37	-11	0.0248	-7470A	PPB	26 Feb 2021 10:44:04	U	SMPL
M1475-02DUP - 1	WA-CONDUP	216	0.0792	-7470A	PPB	26 Feb 2021 10:46:56	U	SMPL
M1475-02MS - 1	WA-CONMS	15405	3.7159	-7470A	PPB	26 Feb 2021 10:49:11	U	SMPL
M1475-02MSD - 1	WA-CONMSD	15766	3.8024	-7470A	PPB	26 Feb 2021 10:51:26	U	SMPL
M1476-02 - 1	ML-CON	-26	0.0212	-7470A	PPB	26 Feb 2021 10:53:42	U	SMPL
M1477-03 - 1	72-11995	17	0.0315	-7470A	PPB	26 Feb 2021 10:55:59	U	SMPL
PB134819TB - 1	PB134802TB	29	0.0344	-7470A	PPB	26 Feb 2021 10:58:15	U	SMPL
M1475-02LX5 - 1		53	0.0402	-7470A	PPB	26 Feb 2021 11:00:31	U	SMPL
M1475-02A - 1		15932	3.8421	-7470A	PPB	26 Feb 2021 11:02:49	U	SMPL
CCV38 - 1	CCV38	20736	4.9924	-7470A	PPB	26 Feb 2021 11:05:06	U	SMPL
CCB38 - 1	CCB38	-34	0.0193	-7470A	PPB	26 Feb 2021 11:07:21	U	SMPL